

45

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
18 May 2007 (18.05.2007)

PCT

(10) International Publication Number
WO 2007/054935 A2

(51) International Patent Classification:

G01T 1/161 (2006.01) G01T 1/29 (2006.01)
G01T 1/166 (2006.01)

(21) International Application Number:

PCT/IL2006/001291

(22) International Filing Date:

9 November 2006 (09.11.2006)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

PCT/IL2005/001173

9 November 2005 (09.11.2005) IL

PCT/IL2005/001215

16 November 2005 (16.11.2005) IL

172349 27 November 2005 (27.11.2005) IL

60/741,440 2 December 2005 (02.12.2005) US

60/750,287 13 December 2005 (13.12.2005) US

60/750,597 15 December 2005 (15.12.2005) US

60/750,334 15 December 2005 (15.12.2005) US

60/754,199 28 December 2005 (28.12.2005) US

PCT/IL2006/000059

15 January 2006 (15.01.2006) IL

60/763,458 31 January 2006 (31.01.2006) US

PCT/IL2006/000562 11 May 2006 (11.05.2006) IL

60/799,688 11 May 2006 (11.05.2006) US

60/800,845 17 May 2006 (17.05.2006) US

60/800,846 17 May 2006 (17.05.2006) US

60/816,970 28 June 2006 (28.06.2006) US

PCT/IL2006/000834 19 July 2006 (19.07.2006) IL

PCT/IL2006/000840 19 July 2006 (19.07.2006) IL

(72) Inventors; and

(75) Inventors/Applicants (for US only): ROUSSO, Benny [IL/IL]; 12 Henri Bergson Street, 75801 Rishon-lezion (IL). ZIV, Omer [IL/IL]; 3 Einstein Street, 76470 Rechovot (IL). NAGLER, Michael [IL/IL]; 4 Avshalom Haviv Street, 69495 Tel-aviv (IL). BEN-HAIM, Shlomo [IL/IL]; 8 Efroni Street, 38900 Caesarea (IL).

(74) Agents: G. E. EHRLICH (1995) LTD. et al.; 11 Menachem Begin Street, 52 521 Ramat Gan (IL).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LV, LY, MA, MD, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— without international search report and to be republished upon receipt of that report

(71) Applicant (for all designated States except US): SPECTRUM DYNAMICS LLC [US/US]; 30 Ramland Road South, Orangeburg, New York 10962 (US).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: DYNAMIC SPECT CAMERA

(57) Abstract: A dynamic SPECT camera is provided, comprising, a plurality of single-pixel detectors, a timing mechanism, in communication with each single-pixel detector, configured for enabling time-binning of the radioactive emissions impinging upon each single-pixel detector to time periods not greater than substantially 30 seconds, and a position-tracker, configured for providing information on the position and orientation of each detecting unit, with respect to the overall structure, substantially at all times, during the individual motion, the dynamic SPECT camera being configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter. The dynamic camera is configured for very short damping time, and may further acquire images in a stationary mode, with no motion. It is further configured for time binning at dynamically varying time-bin lengths, dynamically determining a spectral energy bin for each detecting unit, and employing an anatomic construction of voxels in the imaging and reconstruction.

WO 2007/054935 A2



DYNAMIC SPECT CAMERA

FIELD OF THE INVENTION

The present invention relates SPECT nuclear imaging, and particularly, to systems, methods, and cameras for single-photon-emission-computed-tomography, in list
5 mode, with sensitivity which meets, even outperforms that of PET, in terms of speed and spatial resolution, and with a high spectral resolution not available in PET.

BACKGROUND OF THE INVENTION

Radionuclide imaging aims at obtaining an image of a radioactively labeled
10 substance, that is, a radiopharmaceutical, within the body, following administration, generally, by injection. The substance is chosen so as to be picked up by active pathologies to a different extent from the amount picked up by the surrounding, healthy tissue in consequence, the pathologies are operative as radioactive-emission sources and may be detected by radioactive-emission imaging. A pathology may appear as a
15 concentrated source of high radiation, that is, a hot region, as may be associated with a tumor, or as a region of low-level radiation, which is nonetheless above the background level, as may be associated with carcinoma.

A reversed situation is similarly possible. Dead tissue has practically no pick up of radiopharmaceuticals, and is thus operative as a cold region.

20 The mechanism of localization of a radiopharmaceutical in a particular organ of interest depends on various processes in the organ of interest such as antigen-antibody reactions, physical trapping of particles, receptor site binding, removal of intentionally damaged cells from circulation, and transport of a chemical species across a cell membrane and into the cell by a normally operative metabolic process. A summary of
25 the mechanisms of localization by radiopharmaceuticals is found in <http://www.lunis.luc.edu/nucmed/tutorial/radpharm/i.htm>.

The particular choice of a radionuclide for labeling antibodies depends upon the chemistry of the labeling procedure and the isotope nuclear properties, such as the number of gamma rays emitted, their respective energies, the emission of other particles
30 such as beta or positrons, the isotope half-life, and the decay scheme.

In PET imaging, positron emitting radio-isotopes are used for labeling, and the imaging camera detects coincidence photons, the gamma pair of 0.511 Mev, traveling in opposite directions. Each coincident detection defines a line of sight, along which annihilation takes place. As such, PET imaging collects emission events, which occurred in an imaginary tubular section enclosed by the PET detectors. A gold standard for PET imaging is PET NH_3 rest myocardial perfusion imaging with N-13-ammonia (NH_3), at a dose level of 740 MBq, with attenuation correction. Yet, since the annihilation gamma is of 0.511 Mev, regardless of the radio-isotope, PET imaging does not provide spectral information, and does not differentiate between radio-isotopes.

In SPECT imaging, primarily gamma emitting radio-isotopes are used for labeling, and the imaging camera is designed to detect the actual gamma emission, generally, in an energy range of approximately 11- 511 KeV. Generally, each detecting unit, which represents a single image pixel, has a collimator that defines the solid angle from which radioactive emission events may be detected.

Because PET imaging collects emission events, in the imaginary tubular section enclosed by the PET detectors, while SPECT imaging is limited to the solid collection angles defined by the collimators, generally, PET imaging has a higher sensitivity and spatial resolution than does SPECT. Therefore, the gold standard for spatial and time resolutions in nuclear imaging are defined for PET. For example, there is a gold standard for PET imaging for at rest myocardial perfusion with N-13-ammonia (NH_3), at a dose of 740 MBq with attenuation correction."

Conventional SPECT cameras generally employ an Anger camera, in which a single-pixel scintillation detector, such as NaI(Tl), LSO, GSO, CsI, CaF, or the like, is associated with a plurality of photomultipliers. Dedicated algorithms provide a two dimensional image of the scintillations in the single pixel scintillation detector. There are several disadvantages to this system, for example:

1. the dedicated algorithms associated with the single pixel cannot reach the accuracy of a two-dimensional image of a plurality of single pixel detectors;
2. the single-pixel detector is a rigid unit, which does not have the flexibility of motion of a plurality of small detectors, each with independent motion; and

3. a single hot spot may cause the single pixel detector of the Anger camera to saturate, whereas when a plurality of single pixel detectors is employed, saturation is localized to a few pixels and does not affect the whole image.

Other SPECT cameras which employ a plurality of single pixel detectors are also
5 known.

US Patent 6,628,984, to Weinberg, issued on September 30, 2003 and entitled, "Hand held camera with tomographic capability," describes a tomographic imaging system, which includes a moveable detector or detectors capable of detecting gamma radiation; one or more position sensors for determining the position and angulation of the
10 detector(s) in relation to a gamma ray emitting source; and a computational device for integrating the position and angulation of the detector(s) with information as to the energy and distribution of gamma rays detected by the detector and deriving a three dimensional representation of the source based on the integration. A method of imaging a radiation emitting lesion located in a volume of interest also is disclosed.

15 US Patent 6,242,743, to DeVito, et al., issued on June 5, 2001 and entitled, "Non-orbiting tomographic imaging system," describes a tomographic imaging system which images ionizing radiation such as gamma rays or x rays and which: 1) can produce tomographic images without requiring an orbiting motion of the detector(s) or collimator(s) around the object of interest, 2) produces smaller tomographic systems with
20 enhanced system mobility, and 3) is capable of observing the object of interest from sufficiently many directions to allow multiple time-sequenced tomographic images to be produced. The system consists of a plurality of detector modules which are distributed about or around the object of interest and which fully or partially encircle it. The detector modules are positioned close to the object of interest thereby improving spatial resolution
25 and image quality. The plurality of detectors view a portion of the patient or object of interest simultaneously from a plurality of positions. These attributes are achieved by configuring small modular radiation detector with high-resolution collimators in a combination of application-specific acquisition geometries and non-orbital detector module motion sequences composed of tilting, swiveling and translating motions, and
30 combinations of such motions. Various kinds of module geometry and module or collimator motion sequences are possible, and several combinations of such geometry

and motion are shown. The geometric configurations may be fixed or variable during the acquisition or between acquisition intervals. Clinical applications of various embodiments of US Patent 6,242,743 include imaging of the human heart, breast, brain or limbs, or small animals. Methods of using the non-orbiting tomographic imaging system are also included.

US Patent 5,939,724, to Eisen, et al., issued on August 17, 1999, and entitled, "Light weight-camera head and-camera assemblies containing it," describes a light weight gamma-camera head and assemblies and kits which embody it. The gamma-camera head has a detector assembly which includes an array of room temperature, solid state spectroscopy grade detectors each associated with a collimator and preamplifier, which detectors and associated collimators and preamplifiers are arranged in parallel rows extending in a first direction and suitably spaced from each other in a second direction normal to the first direction, each of the parallel detector rows holding a plurality of detectors. The head may optionally have an electric motor for moving the detector in the second direction and optionally also in the first direction, either stepwise or continuously.

US Patent 6,525,320, to Juni, issued on February 25, 2003, and entitled, Single photon emission computed tomography system, describes a single photon emission computed tomography system, which produces multiple tomographic images of the type representing a three-dimensional distribution of a photon-emitting radioisotope. The system has a base including a patient support for supporting a patient such that a portion of the patient is located in a field of view. A longitudinal axis is defined through the field of view. A detector module is adjacent the field of view and includes a photon-responsive detector. The detector is an elongated strip with a central axis that is generally parallel to the longitudinal axis. The detector is operable to detect if a photon strikes the detector. The detector can also determine a position along the length of the strip where a photon is detected. A photon-blocking member is positioned between the field of view and the detector. The blocking member has an aperture slot for passage of photons aligned with the aperture slot. The slot is generally parallel to the longitudinal axis. A line of response is defined from the detector through the aperture. A displacement device moves either the detector module or the photon-blocking member relative to the other so that the aperture

is displaced relative to the detector and the line of response is swept across at least a portion of the field of view.

US Patent 6,271,525, to Majewski, et al., issued on August 7, 2001, and entitled, "Mini gamma camera, camera system and method of use," describes a gamma camera, which comprises essentially and in order from the front outer or gamma ray impinging surface: 1) a collimator, 2) a scintillator layer, 3) a light guide, 4) an array of position sensitive, high resolution photomultiplier tubes, and 5) printed circuitry for receipt of the output of the photomultipliers. There is also described, a system wherein the output supplied by the high resolution, position sensitive photomultiplier tubes is communicated to: a) a digitizer and b) a computer where it is processed using advanced image processing techniques and a specific algorithm to calculate the center of gravity of any abnormality observed during imaging, and c) optional image display and telecommunications ports.

US Patent 6,271,524, to Wainer, et al., issued on August 7, 2001 and entitled, "Gamma ray collimator," describes a gamma ray collimator assembly comprising collimators of different gamma ray acceptance angles. For example, the acceptance angle of a first collimator may be between 0.2 and 5 degrees, and the acceptance angle of a second collimator may be between about 5 and 30 degrees.

US Patent 6,212,423, to Krakovitz, issued on April 3, 2001 and entitled, "Diagnostic hybrid probes," describes a hybrid nuclear and ultrasonic probe, comprising a cylindrical outer casing surrounding a nuclear probe, which comprises two scintillator plates intersecting perpendicularly, each of the scintillator plates having a plurality of parallel collimators; and an ultrasonic probe situated between said casing at the intersection of said scintillator plates.

List mode data acquisition is known in PET studies, and enables the determination of coincidence. It relates to recording every radiation event together with data pertinent to that event, which includes:

- i. the time the radiation event impinged upon a detector pixel, with respect to a clock, with respect to a time bin, or with respect to another time definition, for example, a time interval between two clock signals; and

ii. the detector pixel location with respect to a coordinate system, at the time of the impinging.

The knowledge of time and location enables the determination of coincidence counts, namely photon counts that arrive substantially simultaneously, 180 degrees apart.

5 The time and location data may be stamped onto the radiation-event data packet, for example, as a header or as a footer, or otherwise associated with the radiation-event data packet, as known.

The time-stamped data available in PET studies may further be used for perfusion studies, where the timing of physiological processes of short durations, that is, durations
10 shorter than about half the time span between heartbeats, is important. Perfusion studies usually involve a sequence of continuous acquisitions, each of which may represent data acquisition duration of about 10 – 30 seconds, although longer durations are sometimes employed. Data from each of the frames is independently reconstructed to form a set of images which can be visualized and used to estimate physiological parameters. This
15 approach involves selection of the set of acquisition times, where one must choose between collecting longer scans with good counting statistics but poor temporal resolution, or shorter scans that are noisy but preserve temporal resolution.

US Patent Application 2003010539, to Tumer, et al., published on June 5, 2003, and entitled, "X-ray and gamma ray detector readout system," describes a readout
20 electronics scheme, under development for high resolution, compact PET (positron emission tomography) imagers, using time tagging, based on LSO (lutetium ortho-oxysilicate, Lu.sub.2SiO.sub.5) scintillator and avalanche photodiode (APD) arrays.

There is some work relating to timing data in SPECT systems, employing Anger cameras.

25 US Patent 5,722,405, to Goldberg, issued on March 3, 1998, and entitled, "Method and apparatus for acquisition and processing of event data in semi list mode," describes a system for acquisition, processing and display of gated SPECT imaging data for use in diagnosing Coronary Artery Disease (CAD) in nuclear medicine, employing an Anger camera, and provides a physician with two parameters for evaluating CAD:
30 information relating to the distribution of blood flow within the myocardium (perfusion) and information relating to myocardium wall motion (function). One aspect provides the

physician with a display of functional images representing quantitative information relating to both perfusion and function with respect to selected regions of interest of the subject heart at end-diastole and end-systole segments of the cardiac cycle. The functional display consists of arcs of varied width depending on wall motion and color coded to illustrate degrees of myocardial perfusion for different pie shaped sections of a selected region of interest within a given short axis slice of reconstructed volume data. Another aspect provides a series of display images allowing facilitated access, display, and comparison of the numerous image frames of the heart that may be collected during gated SPECT sessions. US Patent 5,722,405 also teaches the ability to define and recall parameter files representative of data acquisition and processing parameters and protocol for use in gated SPECT studies and includes a semi-list processing mode to increase efficiency of data acquisition within a camera computer system.

US Patent 7,026,623, to Oaknin, et al., issued on April 11, 2006, and entitled, "Efficient single photon emission imaging," describes a method of diagnostic imaging in a shortened acquisition time for obtaining a reconstructed diagnostic image of a portion of a body of a human patient who was administered with dosage of radiopharmaceutical substance radiating gamma rays, using SPECT and an Anger camera. The method comprises acquiring photons emitted from said portion of the body, by means of a detector capable of converting the photons into electric signals, wherein the total time of photon acquiring is substantially shorter than the clinically acceptable acquisition time; processing said electric signals by a position logic circuitry and thereby deriving data indicative of positions on said photon detector crystal, where the photons have impinged the detector; and reconstructing an image of a spatial distribution of the pharmaceutical substance within the portion of the body by iteratively processing said data. For example, the method includes effective acquisition time of less than 10 minutes, or less than 8 minutes, and acquiring photons in a list-mode procedure.

SUMMARY OF THE INVENTION

The present invention relates to a dynamic SPECT camera, which comprises, a plurality of single-pixel detectors, a timing mechanism, in communication with each single-pixel detector, configured for enabling time-binning of the radioactive emissions

impinging upon each single-pixel detector to time periods not greater than substantially 30 seconds, and a position-tracker, configured for providing information on the position and orientation of each single-pixel detector, with respect to the overall structure, substantially at all times, during the individual motion, the dynamic SPECT camera being
5 configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter. The dynamic camera is further configured for very short damping time, when in stop and shoot acquisition mode and may further acquire images in a stationary mode, with no motion. It is further
10 configured for time binning at dynamically varying time-bin lengths, dynamically determining a spectral energy bin for each single-pixel detector, and constructing and employing an anatomic system of voxels in the imaging and reconstruction.

Unless otherwise defined, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this
15 invention belongs. Although methods and materials similar or equivalent to those described herein can be used in the practice or testing of the present invention, suitable methods and materials are described below. In case of conflict, the patent specification, including definitions, will control. In addition, the materials, methods, and examples are illustrative only and not intended to be limiting.

20 Implementation of the method and system of the present invention involves performing or completing selected tasks or steps manually, automatically, or a combination thereof. Moreover, according to actual instrumentation and equipment of preferred embodiments of the method and system of the present invention, several selected steps could be implemented by hardware or by software on any operating system
25 of any firmware or a combination thereof. For example, as hardware, selected steps of the invention could be implemented as a chip or a circuit. As software, selected steps of the invention could be implemented as a plurality of software instructions being executed by a computer using any suitable operating system. In any case, selected steps of the method and system of the invention could be described as being performed by a data processor,
30 such as a computing platform for executing a plurality of instructions.

BRIEF DESCRIPTION OF THE DRAWINGS

The invention is herein described, by way of example only, with reference to the accompanying drawings. With specific reference now to the drawings in detail, it is stressed that the particulars shown are by way of example and for purposes of illustrative discussion of the preferred embodiments of the present invention only, and are presented in the cause of providing what is believed to be the most useful and readily understood description of the principles and conceptual aspects of the invention. In this regard, no attempt is made to show structural details of the invention in more detail than is necessary for a fundamental understanding of the invention, the description taken with the drawings making apparent to those skilled in the art how the several forms of the invention may be embodied in practice.

In the drawings:

Figures 1A – 1D schematically illustrate a dynamic SPECT camera, in accordance with embodiments of the present invention;

Figures 2A and 2B schematically illustrate the camera structure with the assemblies, in accordance with an embodiment of the present invention.

Figures 3A – 3D schematically illustrate viewing positions, in accordance with embodiments of the present invention.

Figures 4A – 4F schematically illustrate stereo views and cross views, in accordance with embodiments of the present invention.

Figures 5A and 5B illustrate experimental radiopharmaceutical data, as known;

Figures 5C – 5F illustrate cardiac gating, in accordance with embodiments of the present invention;

Figure 6A – 6I illustrate an intracorporeal dynamic SPECT camera, in accordance with embodiments of the present invention;

Figure 7 illustrates assembly damping parameters, in accordance with embodiments of the present invention;

Figures 8A and 8B schematically illustrate grid and anatomical constructions of voxels, in accordance with embodiments of the present invention;

Figures 9A – 9J present experimental data, obtained by the dynamic SPECT camera, in accordance with embodiments of the present invention;

Figure 10 presents experimental data, obtained by the dynamic SPECT camera, in accordance with embodiments of the present invention;

Figures 11 illustrates components of the dynamic SPECT camera, in accordance with embodiments of the present invention; and

5 Figure 12 illustrates an electrical scheme, in accordance with embodiments of the present invention.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

The present invention relates to a dynamic SPECT camera, which comprises, a
10 plurality of single-pixel detectors, a timing mechanism, in communication with each single-pixel detector, configured for enabling time-binning of the radioactive emissions impinging upon each single-pixel detector to time periods not greater than substantially 30 seconds, and a position-tracker, configured for providing information on the position and orientation of each single-pixel detector, with respect to the overall structure,
15 substantially at all times, during the individual motion, the dynamic SPECT camera being configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter. The dynamic camera is further configured for very short damping time, when in stop and shoot acquisition mode
20 and may further acquire images in a stationary mode, with no motion. It is further configured for time binning at dynamically varying time-bin lengths, dynamically determining a spectral energy bin for each single-pixel detector, and constructing and employing an anatomic system of voxels in the imaging and reconstruction.

The principles and operation of the dynamic SPECT camera according to aspects
25 of the present invention may be better understood with reference to the drawings and accompanying descriptions.

Before explaining at least one embodiment of the invention in detail, it is to be understood that the invention is not limited in its application to the details of construction and the arrangement of the components set forth in the following description or illustrated
30 in the drawings. The invention is capable of other embodiments or of being practiced or carried out in various ways. Also, it is to be understood that the phraseology and

terminology employed herein is for the purpose of description and should not be regarded as limiting.

DYNAMIC SPECT CAMERA

5 Design Description of the Dynamic SPECT Camera

An aspect of the present invention relates to a dynamic SPECT camera, with temporal and spatial resolutions which meet, even outperform those of PET, and with a high spectral resolution not available in PET.

10 Temporal resolution, as used herein, relates to a minimal acquisition time for a tomographic reconstruction image of a predetermined volume, for example 15 X 15 X 15 cubic centimeters, and predetermined spatial resolution, for example, 10 X 10 X 10 cubic millimeters. The minimal acquisition time may be, for example, 30 seconds, 10 seconds, or 1 second.

Reference is now made to Figures 1A – 1D, which schematically illustrate a
15 dynamic SPECT camera 10, in accordance with embodiments of the present invention. The dynamic SPECT camera 10 comprises:

- an overall structure 15, which defines proximal and distal ends and, with respect to a body 100;

- a first plurality of assemblies 20, for example, 6, 9, or 16 assemblies 20, arranged
20 on the overall structure 15, forming an array 25 of the assemblies 20, each assembly 20 comprising:

- a second plurality of detecting units 12, each detecting unit 12 including:
 - a single-pixel detector 14, for detecting radioactive emissions; and
 - a dedicated collimator 16, attached to the single-pixel detector 14,
- 25 at the proximal end thereof, for defining a solid collection angle δ for the detecting unit 12.

Additionally, each assembly 20 comprises an assembly motion provider 40, configured for providing the assembly 20 with individual assembly motion, with respect to the overall structure 15, during the acquisition of radioactive-emission data for a
30 tomographic image.

The dynamic SPECT camera 10 further includes:

a timing mechanism 30, in communication with each single-pixel detector 14, configured for enabling time-binning of the radioactive emissions impinging upon each single-pixel detector 14 to time periods not greater than substantially 30 seconds; and

5 a position tracker 50, configured for providing information on the position and orientation of each detecting unit 12, with respect to the overall structure 15, substantially at all times, during the individual assembly motion.

The dynamic SPECT camera 10 is configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, for
10 example, of a target organ 110, such as a heart or a stomach, during an acquisition period no greater than 300 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeters.

It will be appreciated that the time period may be no greater than 200 seconds, 100 seconds, 60 seconds, 30 seconds, 10 seconds, or 1 second.

15 Additionally, the dynamic SPECT camera 10 is configured for acquiring a series of tomographic reconstruction images of a region of interest, as a function of time, at a rate of at least a tomographic reconstruction image every 300 seconds.

Again, the rate may further be every 200 seconds, 100 seconds, 60 seconds, 30 seconds, 10 seconds, or 1 second.

20 In accordance with embodiments of the present invention, the individual assembly motion may be, for example, an assembly oscillatory sweeping motion, as described by an arrow 60. Additionally or alternatively, the individual assembly motion may be a first oscillatory lateral motion, as described by an arrow 80. Additionally or alternatively, the individual assembly motion may be a second oscillatory lateral motion, orthogonal to the
25 first, as described by an arrow 90. Thus, the assembly motion provider 40 may comprise between one and three motion providing units, for the different assembly motions.

Alternatively, the individual assembly motion is an assembly oscillatory sweeping motion, as described by an arrow 60, while the array 25 moves with either the first or the second oscillatory lateral motions, described by the arrows 80 and 90, or with both.

30 Additionally, the detecting units 12 may be grouped into square or rectangular blocks 18, for example, of 4 X 4 detecting units 12, as seen in Figure 1A, or of 16 X 16,

64 X 64, 64 X 128 or another number of detecting units 12. Furthermore, the blocks 18 may be provided with individual block oscillatory sweeping motion, as described by an arrow 70, with respect to the overall structure 15, during the acquisition of radioactive-emission data for a tomographic image. Preferably, the block oscillatory sweeping motion is orthogonal to, or at an angle to the assembly oscillatory sweeping motion, described by the arrow 60. Thus, the assembly motion provider 40 may further comprise a dedicated block motion providing unit, in communication with each block of an assembly.

A control unit 55 may be integrated with the dynamic SPECT camera 10, so as to form a single physical unit, or in communication with the dynamic SPECT camera 10.

A spectral selection mechanism 56, in communication with each of the detecting unit 12, is discussed hereinbelow, under the heading, "dynamically varying spectral bins."

The body 100 may be a human or an animal, and the region of interest, or the target organ 110 may be a heart, a brain, a breast, a stomach, a GI tract, a colon, a prostate, a uterus, a cervix, a vagina, a throat, a gland, a lymph node, a portion of skin, a portion of bone, portion of another tissue, or another body portion.

As seen in Figures 1A and 1B, a reference x;y;z coordinate system illustrates a preferred orientation of the dynamic SPECT camera 10 with respect to the body 100, wherein z runs along a length of the body 100. For convenience, the assembly axis along the assembly length will be referred to as the assembly longitudinal axis, and the assembly axis along the assembly width will be referred to as the assembly traverse axis.

Preferably, the assemblies 20 are long and narrow columns, arranged longitudinally against the body 100, wherein the oscillatory sweeping motion, described by an arrow 60, is about the z-axis. It will be appreciated that other arrangements are similarly possible.

As seen in Figure 1C, illustrating a cross-sectional view in the x-y plane, preferably, the assemblies 20 are arranged in an arc or an arc-like structure, about the body 100, maintaining a shape that follows the body contours, so as to keep as close as possible to the body 100.

Figure 1D provides details of the detecting unit 12. The collimator has a length L , a collection angle δ , and a septa thickness τ . The single pixel detector is preferably a square of sides D and a detector thickness τ_d .

Preferred dimensions for the detecting unit 12 may be, for example, 2.46 mm X 2.46 mm, and the solid collection angle δ may be at least 0.005 steradians. Generally, there may be 16 X 64 detecting units 12 per block 18.

The detector 14 is preferably, a room temperature, solid-state CdZnTe (CZT) detector, which is among the more promising that is currently available. It may be obtained, for example, IMARAD IMAGING SYSTEMS LTD., of Rehovot, ISRAEL, 76124, www.imarad.com, or from eV Products, a division of II-VI Corporation, Saxonburg Pa., 16056, or from or from another source. Alternatively, another solid-state detector such as CdTe, HgI, Si, Ge, or the like, or a combination of a scintillation detector (such as NaI(Tl), LSO, GSO, CsI, CaF, or the like) and a photomultiplier, or another detector as known, may be used, preferably with a photomultiplier tube for each single-pixel detector 14 and collimator 16, for accurate spatial resolution.

Reference is further made to Figures 2A and 2B which schematically illustrate the structure 15 with the assemblies 20, in accordance with an embodiment of the present invention. As seen, the assemblies 20 are arranged in an arc of an angle α , around the body 100, and move in the assembly oscillatory sweeping motion, about the z-axis, so as to provide a plurality of views of the heart 110, from many positions, along the x-y plane.

As seen in Figures 2A and 2B, the dynamic camera 10 is configured for simultaneous acquisition by the assemblies 20, each scanning the same region of interest from a different viewing position, thus achieving both shorter acquisition time and better edge definitions.

Preferably, the structure 15 conforms to the contours of the body 100, so as to maintain substantial contact or near contact with the body.

The embodiment of Figures 2A and 2B illustrate a single type of motion - assembly oscillatory sweeping motion about the z-axis, as described by the arrow 60 (Figure 1A). In some cases, additional motions or views from additional directions may be desirable, as illustrated in Figures 3A - 3D, hereinbelow.

Reference is further made to Figures 3A – 3D, which schematically illustrate viewing positions, in accordance with embodiments of the present invention.

Figure 3A illustrates a cylindrical target organ 110, with a cylindrical radioactive emission source 115 therein.

5 As seen in Figure 3B, a view along the x-axis will observe the cylindrical radioactive emission source 115 as a bar 115.

As seen in Figure 3C, a view along the y-axis will similarly observe the cylindrical radioactive emission source 115 as a bar 115, thus not adding new information to the view along the x axis.

10 It will be appreciated that in the present example, any view along the x-y plane will observe the radioactive emission source 115 as a bar 115.

As seen in Figure 3D, a view along the z-axis will observe the cylindrical radioactive emission source 115 as a circle 115, adding new information to the views along the x and y axes.

15 As Figures 3A – 3D illustrate, at times, views along two axes may be insufficient for a three-dimensional definition of an object, and it may be beneficial to include views with a component along the third axis. For the sake of definition, views along two axis will be referred to stereo views, while views that include a component of the third axis will be referred to as cross views, since they intersect the planer stereo views.

20 Reference is further made to Figures 4A – 4F, which schematically illustrate stereo views and cross views, in accordance with embodiments of the present invention.

Figure 4A illustrate the body 100 with a single assembly 20 arranged for viewing, for example, the heart 110. The assembly 20 is afforded with assembly oscillatory sweeping motion along the z-axis, as described by the arrow 60, and preferably also first and second preferably orthogonal oscillatory lateral motions, described the arrows 80 and 90, respectively.

25 As seen in Figures 4B, the assembly oscillatory sweeping motion along the z-axis, described by the arrow 60, produces views 65 in the x-y planes. The first and second orthogonal oscillatory lateral motions, described the arrows 80 and 90, augment these with additional views 65 in the x-y planes. The purpose of the first and second oscillatory lateral motions is to compensate for “dead areas,” that is, structural areas and

other areas that do not participate in the detection, within the assembly 20 and between the assemblies 20, so as to provide complete coverage of the body 100, by the array 25 (Figure 1A). These motions produce views substantially in the x-y plane. It will be appreciated that there is a component of viewing in a third axis, due to the solid collection
5 angle of the collimator 16. Yet this component is rather small.

Returning to Figure 4A, the blocks 18 of the assembly 20 may be further afforded with block oscillatory sweeping motion, described by the arrow 70 and preferably orthogonal to the assembly oscillatory sweeping motion described by the arrow 60.

As seen in Figure 4C, the block oscillatory sweeping motion, described by the
10 arrow 70, produces cross views 75, which supplement views 65, by providing components of the third axis, namely, the z axis. As illustrated in Figures 3A – 3D, hereinabove, the views 75 may add additional information, not available or barely available in the views 65 along the x-y planes.

Figures 4D and 4F illustrate an alternative mode for acquiring the cross views 75.
15 Accordingly, the dynamic camera 10 further includes assemblies 22, arranged at an angle β to the assemblies 20, and moving with an assembly oscillatory sweeping motion, described by an arrow 62, so as to provide the cross views 75.

The Position Tracker 50

20 The position tracker 50 is configured for providing information on the position and orientation of each detecting unit 12, with respect to the overall structure 15, substantially at all times, during the individual assembly motion.

In accordance with a preferred embodiment of the present invention, the position tracker 50 relates to software and (or) hardware that receive information from the motion
25 provider 40 and calculate the position and orientation of each detecting unit 12, based on that information. Preferably, the calculation is performed within the control unit 55.

Alternatively, position sensors, as known, may be used for determining the position and angular orientation of each detecting unit 12.

Alternatively still, a combination of information from the motion provider 40 and
30 position sensors may be employed.

The Timing Mechanism 30

The timing mechanism 30 associates timing information with the radioactive emission data impinging the single-pixel detectors 14 of the detecting units 12. Preferably the timing mechanism 30 includes a single clock used for all of the single-pixel detectors 14 in the dynamic SPECT camera 10, so that timing information is synchronized for the camera as a whole. The timing information is collected at the single-pixel level, so that time-binning may be performed for the emission data collected by each pixel. Exemplary methods for associating timing information with the radioactive emission data include:

- 1) Time stamping – Each event, impinging on a given single-pixel detector 14 at a given time is stamped with a time of detection and a pixel identification. Stamping may be performed by any manner known in the art, for example as a data packet header or footer. The time-stamped, pixel stamped radioactive emission data may be binned, per time and per pixel, by the control unit 55.
- 2) Time binning – In an alternate approach, timing information is provided for a cumulative count collected from each single-pixel detector 14 over a fixed time interval, for example, 0.001 seconds, 1 second, or 10 seconds, rather than for individual events. Each time bin is then stamped with a time stamp or sequential number and a pixel identification. One technique for performing time binning, is to insert a periodic clock pulse into the data stream. The interval between the clock pulses equals the minimum bin length. Thus, periodic pulses every 0.001 seconds may lead to bin lengths of 0.001 seconds or greater, for example, 1 second, or 10 seconds.

Time Scale Considerations

- Dynamic studies, aimed at obtaining kinetic parameters, require the acquisition of full reconstructed images at a rate that is no greater than about half the frequency of the sampled kinetic parameter. For example, for adult humans, blood circulates through the body at a rate of about 1 cycle per minute. Thus, sampling a process affected by blood circulation should take place at a rate of at least two samplings per minute. Preferably, sampling should be at a much greater rate, for example, 6 samplings or 10 samplings per minute – that is, about every 10 seconds or about every 6 seconds.

Additionally, based on Figures 5A and 5B, according to Garcia et al. (Am. J. Cardiol. 51st Annual Scientific Session, 2002), showing physiological behavior of different radiopharmaceuticals, dynamic studies for Tc-99m teboroxime are best performed within about the first 100 seconds after administration, and better still, within the first 60 seconds after administration.

Moreover, based on Figures 5A and 5B, the dynamic behavior of a radiopharmaceutical in the body, varies as a function of time, depending on the radiopharmaceutical and on the time elapsed since its administration. For example, myocardial perfusion of Tc-99m teboroxime shows a very steep uptake between about the first 10 – 15 seconds and the first 50 – 60 seconds, followed by a more gradual washout, after the first 60 seconds. The rate of sampling of Tc-99m teboroxime, during the first 60 seconds after administration should be adjusted to the very steep uptake, for example, a sampling rate of every second. For radiopharmaceutical with a slower dynamic behavior, a slower rate may be sufficient.

It will be appreciated that a dynamic analysis requires precise knowledge of the time of administration.

Obtaining the Time of Administration of a Radiopharmaceutical

As noted hereinabove, precise knowledge of the time of administration of a radiopharmaceutical is important both in order to evaluate physiological processes made visible by the radiopharmaceutical, with respect to the time of the radiopharmaceutical's entry to the body and in order to perform the evaluation at an optimal period, with respect to the radiopharmaceutical's cycle in the body.

There are several methods for acquiring precise knowledge of the time of administration of the radiopharmaceutical, as follows:

1. providing communication means between an administration device, for example, a syringe or an IV device, and the dynamic SPECT camera 10, and communicating the precise time of administration, vis a vis a clock, by the administration device to the dynamic SPECT camera 10. This method may be employed for example, when administration takes place when the patient is positioned at the dynamic SPECT camera 10, for imaging.

2. providing communication means between the administration device, the dynamic SPECT camera 10, and a third unit, for example, a control system or a hospitals ERP system, communicating the precise time of administration, vis a vis a clock, by the administration device to the third unit, and reporting the precise time of administration by the third unit to the dynamic SPECT camera 10. This method may be employed for example, when administration takes place at a different location than the imaging station.
3. allowing the dynamic SPECT camera 10 to image the site of administration, for example, the arm of the patient, while administration takes place, while employing the timing mechanism 30 of the dynamic SPECT camera 10. A marker, for example, a line of radioactive ink may drawn, for example, on the patient's arm or on the administration device, for defining the time of administration as the time the radiopharmaceutical first crosses the marker. Alternatively, observing a flow of the radiopharmaceutical in the administration device or in the patient's vein may be used to determine the time of administration.
4. Observing a transparent administration device, for example, with a video camera, associated with a clock, may be employed for defining a time of administration based on the radiopharmaceutical distribution in the administration device, or based on the time the radiopharmaceutical first crosses a marker, visible by the video camera. Communication between the video camera and the dynamic SPECT camera 10, or between the video camera, the dynamic SPECT camera 10, and a third unit will provide the information to the dynamic SPECT camera 10.

In accordance with embodiments of the present invention, the administration may include various administration profiles, for example, bolus, continuous drip, or sinusoidal.

Cardiac Gating

The timing mechanism 30 of the dynamic SPECT camera 10 may further be employed for cardiac gating, which is described in detail under a corresponding section, hereinbelow.

When cardiac gating is employed, time binning to time intervals no greater than 50 milliseconds is employed.

Reference is now made to Figures 5C – 5F, which illustrate cardiac gating in accordance with the present invention.

In essence, two different approaches are presented for cardiac gating. In the first, the cardiac RR cycle is divided to a predetermined number of graduations, for example, 16 or 32, so each is of somewhat different time span. In the second, a predetermined graduation time length is chosen, together with an alignment mark for aligning the graduations with a specific state of the RR cycle, and a discard zone is provided, generally around the U-wave region, since the RR cycle may not be exactly divisible by the predetermined graduation time lengths. The cardiac gating may be performed with respiratory gating.

Thus, in accordance with a first embodiment of the present invention, illustrated in Figure 5C, a method of radioactive-emission imaging of a heart is provided, comprising:

imaging the heart of a body, for an imaging period greater than at least 2 cardiac electrical RR cycles 81;

post processing for identifying an average RR interval, based on actual RR time intervals 82, for the body;

post processing for evaluating each specific cardiac electrical cycle, vis a vis the average RR interval, and identifying each of the specific cardiac electrical cycles 81, either as "good," which is to be included in the imaging, or as "bad," for example, due to Arrhythmias, wherein the "bad" cycles are discarded;

dividing each of the "good" cardiac electrical cycles to a fixed number of time graduations 83, for example, 16 or 32;

indexing each graduation 83 with cardiac-cycle indices 84, which associate each graduation with a cardiac-cycle time bin, based on its relative position in the cardiac cycle, for example, with respect to the P-wave, T-Wave, U-wave (see Figure 5F), for example, by assigning a common bin to each P-wave peak, and another common bin to each U-wave dip, and so on; and

adding up photon counts that occurred within the graduations of the same cardiac-cycle bin, from the different "good" RR cycles 81.

Additionally, the method may include performing ECG, concurrent with the imaging, and using the ECG input for identifying durations of the RR intervals 82.

In accordance with an additional embodiment, illustrated in Figure 5D, the method includes:

- 5 extending the imaging period to cover at least two respiratory cycles 85;
- dividing each of the respiratory cycles 85 to respiratory-cycle stages and assigning each of the respiratory-cycle stages a respiratory-cycle index, dividing it into bins, such as bins 86 or 87;
- 10 adding up photon counts that occurred within the graduations of common cardiac-cycle and respiratory-cycle bins, , such as cardiac-cycle index 96 and respiratory index 86, or cardiac-cycle index 97 and respiratory index 87, so as to eliminate respiratory effects.

In accordance with an alternative embodiment, illustrated in Figure 5C, the graduations 83 are fine graduations, and further including:

- 15 amalgamating the fine graduations 83 to coarse graduations 89, wherein each of the coarse graduation 89 includes at least two fine graduations 83;
- indexing each coarse graduation of each of the dedicated graduation time scales with cardiac-cycle indices 91 (analogous to the cycle 84); and
- 20 adding up photon counts that occurred within the coarse graduations 89 of the same cardiac-cycle index bin, for the different "good" RR cycles.

In accordance with an embodiment of the present invention, for each voxel of a reconstructed image, adding up photon counts includes adding up photon counts which occurred within the graduations of the same cardiac-cycle index, for that voxel, from the plurality of detecting units 12.

- 25 Alternatively, for each voxel of a reconstructed image, adding up photon counts includes adding up photon counts which occurred within the graduations of common cardiac-cycle and respiratory-cycle indices, for that voxel, from the plurality of detecting units 12.

- 30 In accordance with another embodiment of the present invention, illustrated in Figure 5E, a method of radioactive-emission imaging of a heart, comprises:

providing a fixed graduation time scale 92, with graduations 93 and at least one graduation mark 94, operative as a point of alignment;

aligning the point of alignment with a specific stage of each of the cardiac electrical cycles, such as "Q," or "R," thus, in effect assigning each one of the cardiac electrical cycles 81 a dedicated one of the graduation time scales 92; and

allowing for a discard zone 95, between adjacent ones of the dedicated graduation time scales 92, where necessary.

Furthermore, the method includes using the ECG input for the aligning of the point of alignment 94 with the specific stage of each of the cardiac electrical cycles, such as "Q," or "R."

It will be appreciated that when stop and shoot acquisition mode is used, the motion of the assemblies 20 is planned to take place during specific portions of the RR cycle.

15 Spatial and Temporal Resolution

In order to meet the time scale considerations, described hereinabove, the dynamic SPECT camera 10 according to embodiments of the present invention is designed at least for acquiring a tomographic reconstruction image of about 15 X 15 X 15 cubic centimeters, which is approximately the volume of a heart, at a predetermined spatial resolution of at least 10 X 10 X 10 cubic millimeters, at an acquisition time no greater than about 30 seconds. Preferably, the acquisition time is no greater than about 10 seconds, and more preferably, the acquisition time is no greater than about 1 second.

Additionally, the spatial resolution of the tomographic reconstruction image may be at least 7 X 7 X 7 cubic millimeters, or better yet, at least 4 X 4 X 4 cubic millimeters, or better still, at least 1 X 1 X 1 cubic millimeters.

When cardiac gating is employed, time binning to time intervals no greater than 50 milliseconds is employed.

Dynamically Varying Time-Bin Lengths

30 There are times when dynamically varying time-bin lengths are desired. For example, Tc-99m-teboroxime has an uptake curve (Figure 5B) which is very steep during

the uptake and which becomes less so during the washout. Thus, different time-bin lengths may be desired for different portions of the Tc-99m-teboroxime uptake curve. Similarly, different radiopharmaceuticals have different uptake curves, and dedicated time-bin lengths may be desired for each radiopharmaceuticals, and for different portions of their respective uptake curves. Moreover, the cardiac RR cycle has very steep periods, during the rise and fall of the R peak (Figure 5F), followed by periods that are nearly flat as a function of time. Again, time bin lengths of different durations may be employed for the different portions of the RR cycle. Furthermore, while the actual region of interest, for example, the heart, requires imaging at a very high level of accuracy, adjacent regions, for example, the chest muscle, may be of lesser interest, and may be viewed at time bins of greater lengths. Additionally, continuous acquisition mode may require shorter time-bin lengths than stop and shoot mode.

For example, the actual rise and fall of the R peak may be gated at time bins of 10 milliseconds, while the nearly levelled U-wave may be gated at 100 milliseconds. Similarly, while the heart muscle may be gated at an average time bin of 50 milliseconds, the adjacent chest muscle may be gated at time bins of 1 second and longer. It will be appreciated that other values may similarly be employed.

In accordance with embodiments of the present invention, a lookup system of recommended time-bin lengths may be provided, for specifying recommended time-bin lengths as functions of at least one of the following:

- a specific region of interest;
- an administered radiopharmaceutical;
- time elapsed since the administration of the radiopharmaceutical;
- cardiac state with respect to an RR cycle;
- a view of the detecting unit 12, with respect to the region of interest;
- patient general data; and
- data acquisition mode.

The lookup system may be, for example, tables or curves.

Thus the dynamic SPECT camera 10 may be configured for time binning at dynamically varying time-bin lengths, by providing communication between the timing

mechanism 30 and the lookup system, wherein the timing mechanism is configured for selecting a recommended time-bin length from the lookup system, for each time bin.

Dynamically Varying Spectral Bins

5 It is sometimes of value to image only a specific spectral bin so as to eliminate scatter or contributions from other radiopharmaceuticals. Additionally, it may be of value to image several spectral bins simultaneously, for different radiopharmaceuticals, wherein different groups of detecting units are dedicated to different spectral bins.

Thus, the dynamic SPECT camera 10 may be configured for dynamically determining a spectral energy bin for each detecting unit 12, as follows:

providing a spectral selection mechanism 56 (Figure 1A), for enabling a selection of a spectral energy bin to be used for each detecting unit 12, independently from the other detecting units 12; and

15 a lookup system of recommended spectral energy bin values, as functions of at least one of a specific region of interest, an administered radiopharmaceutical, time since the administration of the radiopharmaceutical, a view of the detecting unit with respect to the region of interest, and patient's details;

wherein the spectral selection mechanism 56 is further configured for dynamically determining the spectral energy bin for each detecting unit, as functions of the specific 20 region of interest, the administered radiopharmaceutical, the time elapsed since the administration of the radiopharmaceutical, the view of the detecting unit with respect to the region of interest, and patients' details, from the lookup system.

The spectral energy bin is designed to include a primary photon energy $\pm 10\%$, or the primary photon energy $\pm 7\%$, or the primary photon energy $\pm 5\%$.

25 Additionally, at least two radiopharmaceuticals may be administered and viewed by different groups of detecting units, each group being configured for a different spectral energy bin, so as to view each radiopharmaceutical in the same region independently of the other radiopharmaceutical.

The spectral selection mechanism may be a hardware unit or a software.

30 The spectral selection may be performed during data acquisition, or later.

Intracorporeal dynamic SPECT Camera

Referring further to the drawings, Figures 6A – 6I describe the dynamic SPECT camera 10 as an intracorporeal dynamic SPECT camera 10, which includes a single assembly 20, preferably configured for oscillatory sweeping motion around its longitudinal axis – the z axis, as described by the arrow 60. The blocks 18 may be further configured for oscillatory sweeping motion in an orthogonal direction, as described by the arrows 70. An end block 18' may be further configured for motion, for example, as described by the arrow 70'. It will be appreciated that other motions are similarly possible, for example, oscillatory lateral motions, or rotational motions. For example, the arrow 90 describes the oscillatory lateral motion along the z axis of the assembly 20.

An ultrasound transducer 45 may be included with the intracorporeal dynamic SPECT camera 10.

Other features of the intracorporeal dynamic SPECT camera 10 are as described for the dynamic SPECT camera 10 of Figures 1A – 1D.

Figure 6A illustrates the intracorporeal dynamic SPECT camera 10 as a single rigid unit, for example, for rectal or vaginal insertion. Figure 6C illustrates the intracorporeal dynamic SPECT camera 10 as having an incorporeal portion 44, an extracorporeal portion 42 and a cable 46, for example, for insertion to the esophagus.

Figures 6F and 6E illustrate motions of the blocks 18, as described by the arrows 70. Figures 6F – 6I illustrate motion of the assembly 20, as described by the arrow 60.

Image Acquisition Modes

In accordance with embodiments of the present invention, several image acquisition modes are available, as follows:

In a continuous acquisition mode, also referred to as fanning, data is acquired while the array, assembly, or block are in continuous motion. Continuous acquisition mode may apply also to oscillatory motions, although strictly speaking there is a momentary pause with each change of direction. This mode leads to some blurring of the data, but it does not require the array, assembly, or block to stabilize between periods of motion and periods of stationary data acquisition.

In a stop and shoot acquisition mode, incremental travels are followed by stationary acquisition intervals. This mode leads to better resolution, yet it requires a damping period, to allow the array, assembly, or block to stabilize between periods of motion and periods of stationary data acquisition, as discussed hereinbelow, under the heading, "Stability and Damping Time".

Interlacing is a fast stop and shoot acquisition mode with oscillatory motion, for example, sweeping oscillatory motion, wherein on rather than stopping at each predetermined locations, with each sweep, the odd locations are visited on a right sweep and the even locations are visited on the left sweep, or vice versa, so that each sweeping direction stops at different locations.

Prescanning relates to a fast prescan of a subject undergoing diagnosis, to identify a region-of-interest, and thereafter collect higher quality data from the region-of-interest. A prescan according to the present invention may be performed by the dynamic SPECT camera 10, preferably, with interlacing, or in a continuous mode, or by any other imaging device, including, for example, ultrasound or MRI.

Stability and Damping Time

Stop and shoot acquisition mode involves discontinuities in motion between travel and shooting modes, and at the beginning of each shooting mode, the assemblies 20 must be allowed to stabilize till vibrations are less than about ± 0.25 mm, so as not to interfere with the acquisition.

Prior art SPECT cameras must allow for a damping time of about 5 seconds, but the dynamic SPECT camera 10, according to embodiments of the present invention reaches stability in about 1 second or less.

Figure 7 schematically illustrate the assembly 20, according to embodiments of the present invention. The damping time for the assembly 20 may be described as:

$$\text{Damping Time} = C \times \left[(1/12) M (T^2 + W^2) + M X_0^2 \right],$$

wherein:

M is the mass of the assembly 20;

T is the thickness of the assembly 20;

W is the width of the assembly 20;

X_0 is the axis of rotation; and

C is a constant that depends on the braking force applied to the assembly 20.

The factor $1/12$ is calculated assuming the assembly proximal end is tangential to the sweeping path.

5 As the damping time equation illustrates, the damping time is highly dependent on both the axis of rotation X_0 and the mass of the assembly 20.

In the present case, the axis of rotation is that of the sweeping motion described by the arrow 60 (Figure 1A), which is considerably shorter than an axis of rotation around the body 100.

10 Similarly, the mass of a single assembly is far less than that of a conventional SPECT camera.

Possible values for the assembly 20, according to embodiments of the present invention may be:

Weight of the assembly 20 ≈ 1.5 kg.

15 Thickness of the assembly 20 ≈ 5 cm.

Width of the assembly 20 ≈ 7 cm.

As such, the assembly is designed with a damping time constant of under 50 msec during which vibrations amplitude subsides to under .25mm.

20 It will be appreciated that the present example applies to both extracorporeal and intracorporeal dynamic cameras.

Stationary Dynamic SPECT Camera

It may be desired to perform imaging, especially prescanning with a stationary camera, that is without motion, for the following reasons:

- 25
1. in continuous acquisition mode, the blurring produced by the motion is eliminated;
 2. in stop and shoot acquisition mode, the time spent in motion is avoided, as are the vibrations, associated with the discontinuities between the motions and the stationary intervals.

In general, a stationary camera does not provide sufficient viewing positions and detecting units, yet the camera may be specifically designed to provide those, to a desired level.

Preferably, the assemblies 20 are positioned at optimal positions prior to imaging, and imaging takes place while the camera is stationary.

Thus, in accordance with embodiments of the present invention, there is provided a stationary dynamic SPECT camera 10, which is described herein with reference to Figures 1A – 1D. The stationary dynamic SPECT camera 10 comprises:

the overall structure 15, which defines proximal and distal ends with respect to a body;

the first plurality of the assemblies 20, arranged on the overall structure 15, forming an array 25 of the assemblies 20, each assembly 20 comprising:

a second plurality of detecting units 12, each detecting unit 12 including:

a single-pixel detector 14, for detecting radioactive emissions; and

a dedicated collimator 16, attached to the single-pixel detector, at the proximal end thereof, for defining a solid collection angle δ for the detecting unit; and

an assembly motion provider 40, configured for providing the assembly 20 with individual assembly motion with respect to the overall structure, prior to the acquisition of radioactive-emission data;

a position-tracker 50, configured for providing information on the position and orientation of each of the detecting units 12, with respect to the overall structure 15, during the individual motion,

the stationary dynamic SPECT camera 10 being configured for acquiring a tomographic reconstruction image of a region of interest while stationary, for the whole duration of the tomographic image acquisition.

Preferably, the region of interest is about 15 X 15 X 15 cubic centimeters, and the tomographic image may be acquired during an acquisition time of 60 seconds, at a spatial resolution of at least 20 X 20 X 20 cubic millimeter.

Additionally, the tomographic image may be acquired during an acquisition time of 30 seconds, at a spatial resolution of at least 20 X 20 X 20 cubic millimeter.

Furthermore, the tomographic image may be acquired during an acquisition time of 60 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

Additionally, the tomographic image may be acquired during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

5 Preferably, the structure 15 conforms to the contours of the body 100, for acquisition with substantial contact or near contact with the body.

Additionally, the assemblies 20 in the array 25 are configured to provide stereo views in a plane and cross views.

10 Anatomic Construction of Voxels

Anatomic construction of voxels avoids the smearing effect of a rigid voxel grid construction, where different tissue types, for example, blood and muscle, appear in a same voxel. This is important especially for perfusion studies, where the perfusion of blood into the tissue is sought.

15 Reference is now made to Figures 8A and 8B, which schematically illustrate a rigid voxel grid construction and an anatomic construction of voxels, respectively, in accordance with the present invention.

Figures 8A and 8B illustrate a heart 200, having atria 202 and 204, chambers 206 and 208, and a muscle 218.

20 As seen in Figure 8A, a rigid voxel construction 202 causes smearing of the different tissue types. However, as seen in Figure 8B, blood and muscle tissues are anatomically divided into different voxels, allowing an accurate study of perfusion. The atria and chambers are divided into an anatomic voxel system 222, or to an anatomic voxel system 224, while the muscle is divided into a relatively coarse voxel system 226, 25 or to a finer voxel system 228, as desired. It will be appreciated that the anatomic voxels may vary in volume. For example, since ischemia is not relevant to the atria and chambers, they may be divided into coarse voxels, while the heart muscle may be divided into fine voxels.

30 As further seen in Figure 8B, the rigid voxel construction 202 may still applied to the surrounding chest muscle.

It will be appreciated that parametric equations, such as $F(1)$ and $F(2)$ may be created and used in the construction of the anatomic construction of the voxels.

The following describes methods for obtaining the anatomic construction of voxels.

- 5 A first method for the anatomic construction of voxels includes:
- providing a structural image of a region of interest, such as a heart;
 - constructing an anatomic system of voxels, for the region of interest, in which voxel boundaries are aligned with boundaries of structural objects of the region of interest, based on the structural image;
 - 10 performing radioactive-emission imaging of the region of interest, utilizing the anatomic system of voxels; and
 - performing reconstruction of the radioactive-emission imaging, utilizing the anatomic system of voxels.

15 Preferably, the structural image is provided by a structural imager, selected from the group consisting of 2-D ultrasound, 3-D ultrasound, planner x-rays, CT x-rays, and MRI.

Additionally, the structural imager is co-registered to a radioactive-emission imaging camera which performs the radioactive-emission imaging.

20 Moreover, attenuation correction of the radioactive-emission imaging may be performed, based on the structural image.

Furthermore, the structural image and the radioactive-emission image, constructed with the anatomic voxels, may be displayed together.

25 Alternatively, the structural imager is not co-registered to a radioactive-emission imaging camera which performs the radioactive-emission imaging, and further including corrections for misregistration.

Alternatively still, the structural image is provided from a lookup system, which is preferably corrected for patient's details.

30 It will be appreciated that the anatomic construction of voxels may be based on fitting the boundaries of the structural objects to parametric equations and utilizing the parametric equations in the constructing of the anatomic system of voxels.

Additionally, the anatomic system of voxels includes voxels of varying volumes, depending on their anatomic position and relevance.

Furthermore, the method includes time-binning of the radioactive emissions to time periods not greater than substantially 30 seconds, or not greater than substantially 10 seconds, or not greater than substantially 1 second.

Additionally, the anatomic system of voxels includes voxels of varying volumes, depending on the relevance of their dynamic activity.

An alternative method for the anatomic construction of voxels includes, relates to the use of the radioactive emission imaging itself for the anatomic reconstruction, as follows:

providing a first system of voxels for a region of interest;
obtaining radioactive-emission data from the region of interest;
performing a first reconstruction, based on the radioactive-emission data and the first system of voxels, to obtain a first image;
correcting the first system of voxels, by aligning voxel boundaries with object boundaries, based on the first image; thus obtaining a second system of voxels;
performing a second reconstruction, based on the radioactive-emission data and the second system of voxels, thus obtaining a second image.

Alternatively, a set of radioactive emission data is obtained, possibly with a second injection, in order to concentrate the viewing on the anatomic voxels, as follows:

providing a first system of voxels for a region of interest;
obtaining a first set of radioactive-emission data from the region of interest;
performing a first reconstruction, based on the first set of the radioactive-emission data and the first system of voxels, to obtain a first image;
correcting the first system of voxels, by aligning voxel boundaries with object boundaries, based on the first image; thus obtaining a second system of voxels, which is anatomically based;

obtaining a second set of radioactive-emission data from the region of interest, based on the second system of voxels, which is anatomically based; and

performing a second reconstruction, based on the second set of the radioactive-emission data and the second system of voxels, thus obtaining a second image.

Anatomic Modeling

Bull's Eye, or polar map, is a semi-automatic method for the quantification and evaluation of coronary artery disease from SPECT tomograms obtained by marking the myocardium with Tl-201 or MIBI-Tc-99. The polar map is computed from cross-sectional slices of the Left Ventricle (LV). For each slice, the center and a radius of search that contains the LV are determined and the LV is divided into radial sectors. The maximum count value of each sector is computed, generating a profile. Profiles are plotted as concentric circle onto the map. The resulting map is a compression of 3D information (LV perfusion) onto a single 2D image.

Yet the bull's eye or polar map is reconstructed from a rigorous geometry of voxels, for example, of 5 X 5 X 5 mm, or 4 X 4 X 4 mm, which cuts across tissue types, thus providing smeared information.

A voxel division that is based on an anatomical structure would be highly preferred, as it would allow the measurements of processes within and across anatomical features, substantially without the smearing effect. For example, if specific voxels are used to define blood regions, and others are used to define muscle regions, than diffusion across boundary membranes and other processes may be evaluated, substantially without a smearing effect.

Anatomical model is based on voxels that follow anatomical structures, and may be shaped for example, as a sphere, a tube, or as a shell segment, rather than as a the standard cube.

When combined with a camera of high resolution and sensitivity and with gated measurements, anatomic modeling would be clearly advantageous over standard, rigorous modeling, especially for kinetic studies are meaningful only with respect to specific tissue types.

In accordance with embodiments of the present invention, the polar map may be produced with a reduced number of amplitudes, or levels, for example, 7 levels of severity, or 5 levels of severity, from healthy to severe.

Kinetic Modeling

As part of the imaging and analysis processes, the camera may be able to produce a time series of 2D or 3D images, showing reconstructed intensity in space and its changes over time.

Likewise, it may be desirable not to reconstruct the entire volume but only limited segments of interest. In those segments, resolution of segment definition may be very important in order to minimize partial volume effect, which results in a biased estimate of the kinetic process.

In an exemplary embodiment, the analysis of the kinetic process may be after reconstruction of the intensity in the entire volume or in the selected segments has been done for a series of time points. In that case, each segment or location in space (u) has a list of intensity (I) values in time (t), and the list $I(u,t)$ may be further analyzed to fit parametric kinetic model.

Such a parametric kinetic model may be a variety of kinds, depending on the modeling on the biological process. Examples of such models may be found in PCT/IL2005/001173. In a simplistic example, the model may be

$$I(u,t) = B(t) \bullet \left(1 - e^{-k_1(u) \cdot t}\right) \bullet e^{-k_2(u) \cdot t}$$

where $B(t)$ is a concentration in the blood, whether obtained from imaging a segment which is pure blood (e.g. major blood vessel, or volume within the heart chamber), or may be known from other sources (by injection profile, other invasive or non invasive measurements from the blood, etc). $k_1(u)$ is the time constant representing a process of uptake into the tissue at segment u , and $k_2(u)$ is the time constant representing a process of washout from the tissue at segment u .

There may be many other models, and for example the equation above may take other forms such as

$$I(u,t) = B(t) * F_1(k_1(u), \tau) * F_2(k_2(u), \tau)$$

where $*$ stands for either multiply operation or convolution in most cases, and F_1 and F_2 represent processes. In an example, the effect of such process on the intensity may be modeled in linear cases by convolution of the intensity in the blood with an impulse response of a linear process $F_i(k_i(u), \tau)$. Each of these may include one or more time constants $k_i(u)$, and the time profile is described as a function of time τ . There may be one or more such processes F_i , for example 1 (e.g. uptake or decay only), 2 (e.g. simultaneous uptake and clearance processes), 3 (e.g. combination with accumulation or metabolism), 4 or more.

A process of fitting may be used between the reconstructed intensity in space and time and the parametric models mentioned above.

In another example, the parametric model may be incorporated *into the reconstruction process*. In this case, it is not necessary to perform reconstruction of intensities $I(u, t)$ in space and time and then use that information to extract time constants of biological processes $k_i(u)$.

5 Instead, the imaging equation

$$y_n(t) \sim \text{Poisson}\left(\sum_u \varphi_n(u) I(u, t)\right)$$

10 may be explicitly replaced with the model of the intensities

$$y_n(t) \sim \text{Poisson}\left(\sum_u \varphi_n(u) B(t) * F_1(k_1(u), \tau) * F_2(k_2(u), \tau)\right)$$

15 (where $y_n(t)$ is the number of photon measured from a viewing position n with a probability function of the view $\varphi_n(u)$).

In this case, the reconstruction process (e.g. by Maximum-Likelihood, Expectation maximization, or other equation solving techniques) is used to recover the best fitting values of $k_i(u)$, instead of recovering $I(u, t)$ and then $k_i(u)$.

20 In some embodiments of the present invention, the use of a camera directly intended to perform dynamic studies, the ability to avoid interim recovery of intensities in 3D-space in various time periods may be a benefit, as the design of the scanning is optimized for the kinetic parameters reconstruction, and not necessarily to image quality in each time point.

25

Active Vision

The camera of the present invention may further include active vision which relates to a method of radioactive-emission measurements of a body structure, comprising:

performing radioactive-emission measurements of the body structure, at a predetermined set of views;

analyzing the radioactive-emission measurements; and

dynamically defining further views for measurements, based on the analyzing.

Active vision may be used, for example, to better define an edge, by changing a view direction, to direct a saturating detecting unit away from a hot spot, to change the

duration at a certain location, when a greater number of counts are required, or when sufficient counts have been obtained.

Reconstruction Stabilizer

5 The method of reconstruction employed by the present invention may further include a method for stabilizing the reconstruction of an imaged volume, comprising:

 performing an analysis of the reliability of reconstruction of a radioactive-emission density distribution of said volume from radiation detected over a specified set of views; and

10 defining modifications to at least one of a reconstruction process and a data collection process to improve said reliability of reconstruction, in accordance with said analysis.

 Additionally, the method may include calculating a measure of said reliability of reconstruction, said measure of reliability of reconstruction being for determining a
15 necessity of performing said modifications.

 Furthermore, the method may include:

 providing a detection probability matrix defining a respective detection probability distribution of said volume for each of said views; calculating the singular values of said detection probability matrix;

20 identifying singular values as destabilizing singular values.

 Additionally, the method may include calculating a condition number of said probability matrix as a measure of said reliability of reconstruction.

 It will be appreciated that this approach may result in non-uniform voxels, wherein voxel volume may increase or decrease as necessary to increase the reliability of
25 the reconstruction

View Selection

 The present invention further utilizes a method of optimal view selection, as follows:

30 providing said volume to be imaged;
 modeling said volume;

providing a collection of views of said model;

providing a scoring function, by which any set of at least one view from said collection is scorable with a score that rates information obtained from said volume by said set;

- 5 forming sets of views and scoring them, by said scoring function; and
 selecting a set of views from said collection, based on said scoring function for imaging said volume.

10 Additionally, zooming in onto a suspected pathology may be performed by a two-step view selection, wherein once the suspected pathology is observed, that region of the volume is modeled anew and a new collection of views is obtained specifically for the suspected pathology.

Experimental Results

15 Reference is now made to Figures 9A – 9J, which schematically illustrate cardiac imaging of Tc-99m-Teboroxime, with the dynamic camera 10 in accordance with aspects of the present invention. The significance of the experimental data provided herein is the ability to successfully image Teboroxime, which as Figure 5B illustrates is washed out of the body very quickly.

Figure 9A provides anatomical landmarks, as follows:

- 20 ●Left Ventricle (LV)
 ●Right Ventricle (RV)
 ●Left Atrium (LA)
 ●Right Atrium (RA)

25 Figure 9B is a dynamic study input of bloodpool, myocardium, and body timed activity.

Figure 9C is a Film-stripe representation of a dynamic SPECT study, as follows:

- First 2 minutes after Tc99m-Teboroxime* injection, 10s/frame
- Mid-ventricular slices (upper row : SA lower row: HLA)

30 Note: as the intense blood pool activity at the center of the heart chambers gradually clears, while the myocardial uptake gradually intensifies.

Figure 9D is a Film-stripe representation of a dynamic SPECT study, as follows:

- First 4 minutes after Tc99m-Teboroxime* injection, 10s/frame
- Mid-ventricular slices (upper row : SA lower row: HLA)

Note: as the intense blood pool activity at the center of the heart chambers gradually clears, while the myocardial uptake gradually intensifies

5 Figure 9E is a Movie representation of a dynamic SPECT study (SA), as follows:

- First 4 minutes after Tc99m-Teboroxime* injection, 10s/frame
- Mid-ventricular SA slices.

Note: as the intense blood pool activity gradually clears in LV and RV cavities

Note: Myocardial uptake gradually intensifies, (the thin walled RV is less intense)

10 Figure 9F is a Movie representation of a dynamic SPECT study (SA), as follows:

- First 4 minutes after Tc99m-Teboroxime* injection, 10s/frame
- Mid-ventricular SA slices.

Note: as the intense blood pool activity gradually clears in LV, RV, LA and RA cavities

15 Note: Myocardial uptake gradually intensifies, (the thin walled RV ant atria are less intense)

Figure 9G is a Movie representation of a dynamic SPECT study (fast).

Figure 9H is a Movie representation of a dynamic SPECT study (slow).

20 Figure 9I represents volume segmentation for separate tissue flow dynamics measurement

Figure 9J represents measured kinetic curves.

Figure 10 is another experiment, illustrating time binning at a rate of 0.001 seconds.

25 Electronic Scheme for Fast Throughput

High-sensitivity detecting units, such as the room temperature, solid-state CdZnTe (CZT) detectors utilized in the present embodiments, must be discharged frequently, as their high-sensitivity can lead to rapid saturation. When a given detector saturates, the output count for the associated pixel no longer accurately reflects the number of incoming photons, but rather the maximum number that the detector is capable of absorbing. This

30

inaccuracy may lead to errors during reconstruction. It is therefore important to perform readout often enough to avoid detector saturation.

The data channel from the assembly 20 (or the assembly 20 readout circuitry) to the signal processing components must be fast enough to handle the large quantities of data which are obtained from the detecting units 12.

The electronic scheme of the present embodiments preferably includes one or more of the following solutions for performing frequent detector unit readout, while maintaining high data throughput to prevent data channel saturation.

In a preferred embodiment, the dynamic SPECT camera 10 includes a parallel readout unit for performing parallel readout of emission count data. Parallel readout requires less time than serial readout (in which the pixels are read out in sequence), as multiple pixels may be read out in a single cycle without losing the information of the individual pixel counts. The readout rate can thus be increased without loss of data.

Parallel readout may be performed at many levels. Reference is now made to Figure 11, which illustrates various levels of detector unit organization at which parallel readout may be performed. The present exemplary embodiment shows a single detector array 25, which includes three assemblies 20. Each assembly includes a plurality of blocks 18 of detector units 12. Each detecting unit 12 includes a single-pixel detector (Figure 1D).

The parallel readout unit preferably performs parallel readout at the level of one or more of:

- a) detecting units 12, each of the single-pixel detector 14;
- b) blocks 18, which include a plurality of detecting units 12;
- c) assemblies 20, which include a plurality of blocks 18
- d) array 25, which includes a plurality of assemblies 20.

When the parallel readout unit performs parallel readout at the level of the detecting units 12, count values are read out in parallel from each of the electrically insulated single-pixel detector 14. The single-pixel detector 14 is discharged at readout, and the photon collection process begins anew.

When the parallel readout unit performs parallel readout at the level of the block 18, count values from each of the detecting units 12 are read out serially, however

multiple blocks 18 are read out in parallel. This approach is less complex to implement than parallel readout of the detecting units 12, although it results in a certain reduction in readout rate to accommodate the serial readout. Again, the single-pixel detectors 14 are discharged at readout.

5 Similarly, when the parallel readout unit performs parallel readout at the level of the assembly 20, count values from each of the detecting units 12 in the assembly 20 are read out serially, however multiple assemblies 20 are read out in parallel.

Parallel readout preferably includes multiple detection, amplification and signal processing paths for each of the pixels, thereby avoiding saturation due to a single
10 localized high emission area - "hot spot". This is in contrast with the Anger camera, in which multiple collimators are associated with a single-pixel scintillation detector, and saturation of the scintillation detector may occur even due to a localized hot spot.

Figure 12 illustrates an exemplary embodiment of parallel readout in the dynamic SPECT camera 10. Radioactive emissions are detected by pixelated CZT crystals, where
15 each crystal is divided into 256 pixels. The crystal is part of a 'CZT MODULE' (B) which also includes two ASICS each receiving events from 128 pixels. The ASIC is an OMS 'XAIM3.4' made by Orbotech Medical Systems, Rehovot, Israel, together with the CZT crystal. The 2 ASICs share a common output and transmit the data to 'ADC PCB' (C) that handles four 'CZT MODULES' (B) in parallel. Thus, a total of 1024 pixels are
20 presently channeled through one ADC board. The system is capable of further increasing the accepted event rate by channeling every two ASICS through a single ADC. The 'ADC PCB' (C) transmits the data to the 'NRG PCB' (D) that handles ten 'ADC PCB's' (C) in parallel, but could be further replicated should one want to further decrease "dead time". The 'NRG PCB' (D) transmits the data to the 'PC' (E) where it is stored.

25 All in all, in the present embodiment, forty CZT MODULEs which contain a total of 10240 pixels transmit in parallel to the PC.

The bottle neck, and hence the only constraint, of the system data flow is the ASICS in the 'CZT MODULE' (B) and the connection to the 'ADC PCB's' (C):

1. An ASIC (128 pixels) can process one photon hit within 3.5uSec, or 285,000
30 events/sec over 128 pixels, i.e. over 2200 events/px/sec-an exceedingly high rate.

2. Two ASICS share the same output, and hence coincident event output of the two ASICS in a 'CZT MODULE' (B) will cause a collision and information loss. The duration of an event output from the ASIC is 1uSec.

When the readout is rapid, the rate at which the radiation emission data is read out of the single-pixel detectors 14 may be greater than the rate at which it may be output to the processor. One known solution for managing a difference data arrival and data processing rates is to use a buffer. The buffer provides temporary storage of the incoming data, which is retrieved at a later time.

A buffered readout configuration can result in the loss of timing information, unless active steps are taken to preserve the time information associated with the collected emission data, for example, as taught hereinabove, under the heading, "The Timing Mechanism 30."

In accordance with embodiments of the present invention, timing information is preserved. The electrical scheme may include a buffer which stores emission data along with timing information for each data item or group of data items (in the case where emission data from several detectors was obtained at substantially the same time, for example due to parallel readout), and an identification of the associated detector unit. Utilizing a buffer ensures that emission data may be collected from the detectors frequently enough to avoid saturation, even when the data channel throughput is limited. In stop and shoot mode, for example, the emission count data may be stored in the buffer for retrieval while the detector head is moving to the next location. Accurate reconstruction may thus be performed.

The camera readout circuitry is preferably designed to provide fast readout and detecting unit discharge. Fast readout circuitry may include fast analog and digital circuitry, fast A/D converters, pipelined readout, and so forth.

After the emission data has been read out of the single-pixel detectors 14, it may be necessary to convey the data to a processor for reconstruction as a single or limited number of data streams. The camera electronic scheme may include a multiplexer, for combining two or more emission data streams into a single data stream. The emission data may thus be conveyed to the processor over one physical link (or alternately over a reduced number of parallel links). For each radioactive emission event, the multiplexer

includes both the timing information and an identification of the single-pixel detector 14 supplying the event. The multiplexed data may later be de-multiplexed by the processor, and reconstruction may be performed with complete information for each data item, including for example, total counts per single-pixel detector 14, per time bin, single-pixel
5 detector location and orientation, and the time bin. Parallel readout may thus be performed, even when the collected data is to be output over a single data link.

Sensitivity Consideration.

It will be appreciated that dynamic imaging with a SPECT camera has been
10 attempted in the past, unsuccessfully, primarily, because prior-art SPECT cameras are not sensitive enough to provide tomographic reconstruction images, for example, of a heart, with sufficient object resolution, for example, 10 X 10 X 10 cubic millimeters, in less than a minute.

As a case in point, US Patent 7,026,623, to Oaknin, et al., filed on January 7,
15 2004, issued on April 11, 2006, and entitled, "Efficient single photon emission imaging," describes a method of diagnostic imaging in a shortened acquisition time for obtaining a reconstructed diagnostic image of a portion of a body of a human patient who was administered with dosage of radiopharmaceutical substance radiating gamma rays, using an Anger Camera and SPECT imaging. The method includes effective acquisition times
20 from less than 14 minutes to less than 8 minutes. Oaknin, et al., do not claim an effective acquisition time of less than 7 minutes. Yet, in view of the section entitled, "Time Scale Considerations," hereinabove, a sampling rate of 8 about minutes is far too slow for myocardial perfusion studies, where a sampling rate of at least two tomographic reconstruction images per heartbeat, that is, about every 30 seconds, is desired, and
25 furthermore, where processes occur at rates of several seconds, and must be sampled at rates of a second or less, as seen in Figure 5B.

The dynamic SPECT camera 10 in accordance with embodiments of the present invention achieves sensitivity sufficient for the required sampling rates of between every 30 seconds and every half a second, by combining several features, specifically intended
30 to increase sensitivity, as follows:

a collimator 16 with a solid collection angle δ of at least 0.005 steradians or greater, for a fast collection rate, and high sensitivity, wherein the loss in resolution is compensated by one or a combination of the following factors:

- i. motion in a stop and shoot acquisition mode, at very small incremental steps, of between about 0.01 degrees and about 0.75 degrees.
- ii. simultaneous acquisition by the assemblies 20, each scanning the same region of interest from a different viewing position, thus achieving both shorter acquisition time and better edge definitions.
- iii. the structure 15 conforming to the body contours, for acquisition with substantial contact or near contact with the body.

Definition of a Clinically-Valuable Image

In consequence, the dynamic SPECT camera 10 is capable of producing a "clinically-valuable image" of an intra-body region of interest (ROI) containing a radiopharmaceutical, while fulfilling one or more of the following criteria:

1. the dynamic SPECT camera 10 is capable of acquiring at least one of 5000 photons emitted from the ROI during the image acquisition procedure, such as at least one of 4000, 3000, 2500, 2000, 1500, 1200, 1000, 800, 600, 400, 200, 100, or 50 photons emitted from the ROI. In one particular embodiment, the camera is capable of acquiring at least one of 2000 photons emitted from the ROI during the image acquisition procedure;
2. the dynamic SPECT camera 10 is capable of acquiring at least 200,000 photons, such as at least 500,000, 1,000,000, 2,000,000, 3,000,000, 4,000,000, 5,000,000, 8,000,000, or 10,000,000 photons, emitted from a portion of the ROI having a volume of no more than 500 cc, such as a volume of no more than 500 cc, 400 cc, 300 cc, 200 cc, 150 cc, 100cc, or 50 cc. In one particular embodiment, the camera is capable of acquiring at least 1,000,000 photons emitted from a volume of the ROI having a volume of no more than 200 cc;
3. the dynamic SPECT camera 10 is capable of acquiring an image of a resolution of at least 7x7x7 mm, such as at least 6x6x6 mm, 5x5x5 mm, 4x4x4 mm, 4x3x3 mm, or 3x3x3 mm, in at least 50% of the reconstructed volume, wherein the radiopharmaceutical

as distributed within the ROI has a range of emission-intensities I (which is measured as emitted photons / unit time / volume), and wherein at least 50% of the voxels of the reconstructed three-dimensional emission-intensity image of the ROI have inaccuracies of less than 30% of range I , such as less than 25%, 20%, 15%, 10%, 5%, 2%, 1%, or 0.5% of range I . For example, the radiopharmaceutical may emit over a range from 0 photons/second/cc to 10^5 photons/second/cc, such that the range I is 10^5 photons/second/cc, and at least 50% of the voxels of the reconstructed three-dimensional intensity image of the ROI have inaccuracies of less than 15% of range I , i.e., less than 1.5×10^4 photons/second/cc. For some applications, the study produce a parametric image related to a physiological process occurring in each voxel. In one particular embodiment, the image has a resolution of at least 5x5x5 mm, and at least 50% of the voxels have inaccuracies of less than 15% of range I ;

4. the dynamic SPECT camera 10 is capable of acquiring an image, which has a resolution of at least 7x7x7 mm, such as at least 6x6x6 mm, 5x5x5 mm, 4x4x4 mm, 4x3x3 mm, or 3x3x3 mm, in at least 50% of the reconstructed volume, wherein the radiopharmaceutical as distributed within the ROI has a range of emission-intensities I (which is measured as emitted photons / unit time / volume), and wherein at least 50% of the voxels of the reconstructed three-dimensional emission-intensity image of the ROI have inaccuracies of less than 30% of range I , such as less than 25%, 20%, 15%, 10%, 5%, 2%, 1%, or 0.5% of range I . For example, the radiopharmaceutical may emit over a range from 0 photons/second/cc to 10^5 photons/second/cc, such that the range I is 10^5 photons/second/cc, and at least 50% of the voxels of the reconstructed three-dimensional intensity image of the ROI have inaccuracies of less than 15% of range I , i.e., less than 1.5×10^4 photons/second/cc. For some applications, the study produces a parametric image related to a physiological process occurring in each voxel. In one particular embodiment, the image has a resolution of at least 5x5x5 mm, and at least 50% of the voxels have inaccuracies of less than 15% of range I ;

5. the dynamic SPECT camera 10 is capable of acquiring an image, which has a resolution of at least 20x20x20 mm, such as at least 15x15x15 mm, 10x10x10 mm, 7x7x7 mm, 5x5x5 mm, 4x4x4 mm, 4x3x3 mm, or 3x3x3 mm, wherein values of parameters of a physiological process modeled by a parametric representation have a range of

physiological parameter values I , and wherein at least 50% of the voxels of the reconstructed parametric three-dimensional image have inaccuracies less than 100% of range I , such as less than 70%, 50%, 40%, 30%, 25%, 20%, 15%, 10%, 5%, 2%, 1%, or 0.5% of range I . For example, the physiological process may include blood flow, the values of the parameters of the physiological process may have a range from 0 to 100 cc / minute, such that the range I is 100 cc / minute, and at least 50% of the voxels of the reconstructed parametric three-dimensional image have inaccuracies less than 25% of range I , i.e., less than 25 cc / minute. In one particular embodiment, the image has a resolution of at least 5x5x5 mm, and at least 50% of the voxels have inaccuracies of less than 25% of range I ; and/or

6. the dynamic SPECT camera 10 is capable of acquiring an image, which has a resolution of at least 7x7x7 mm, such as at least 6x6x6 mm, 5x5x5 mm, 4x4x4 mm, 4x3x3 mm, or 3x3x3 mm, in at least 50% of the reconstructed volume, wherein if the radiopharmaceutical is distributed substantially uniformly within a portion of the ROI with an emission-intensity $I \pm 10\%$ (which is defined as emitted photons / unit time / volume), and wherein at least 85% of the voxels of the reconstructed three-dimensional emission-intensity image of the portion of the ROI have inaccuracies of less than 30% of intensity I , such as less than 15%, 10%, 5%, 2%, 1%, 0.5%, 20%, or 25% of intensity I . For example, the radiopharmaceutical may be distributed within a volume with a uniform emission-intensity I of 10^5 photons/second/cc, and at least 85% of the voxels of the reconstructed three-dimensional intensity image of the volume have inaccuracies of less than 15% of intensity I , i.e., less than 1.5×10^4 photons/second/cc. For some applications, the same definition may apply to a study which produces a parametric image related to a physiological process occurring in each voxel. In one particular embodiment, the image has a resolution of at least 5x5x5 mm, and at least 50% of the voxels have inaccuracies of less than 15% of intensity I .

It is expected that during the life of this patent many relevant dynamic SPECT cameras will be developed and the scope of the term dynamic SPECT camera is intended to include all such new technologies *a priori*.

As used herein the term "substantially" refers to $\pm 10\%$.

As used herein the term "about" refers to $\pm 30\%$.

Additional objects, advantages, and novel features of the present invention will become apparent to one ordinarily skilled in the art upon examination of the following examples, which are not intended to be limiting. Additionally, each of the various
5 embodiments and aspects of the present invention as delineated hereinabove and as claimed in the claims section below finds experimental support in the following examples.

It is appreciated that certain features of the invention, which are, for clarity, described in the context of separate embodiments, may also be provided in combination in a single embodiment. Conversely, various features of the invention, which are, for
10 brevity, described in the context of a single embodiment, may also be provided separately or in any suitable subcombination.

Although the invention has been described in conjunction with specific embodiments thereof, it is evident that many alternatives, modifications and variations will be apparent to those skilled in the art. Accordingly, it is intended to embrace all such
15 alternatives, modifications and variations that fall within the spirit and broad scope of the appended claims. All publications, patents and patent applications mentioned in this specification are herein incorporated in their entirety by reference into the specification, to the same extent as if each individual publication, patent or patent application was specifically and individually indicated to be incorporated herein by reference. In addition,
20 citation or identification of any reference in this application shall not be construed as an admission that such reference is available as prior art to the present invention.

What is claimed:

1. A dynamic SPECT camera, comprising:
 - an overall structure, which defines proximal and distal ends with respect to a body;
 - a first plurality of assemblies, arranged on the overall structure, forming an array of the assemblies, each assembly comprising:
 - a second plurality of detecting units, each detecting unit including:
 - a single-pixel detector, for detecting radioactive emissions; and
 - a dedicated collimator, attached to the single-pixel detector, at the proximal end thereof, for defining a solid collection angle δ for the detecting unit; and
 - an assembly motion provider, configured for providing the assembly with individual assembly motion with respect to the overall structure, during the acquisition of radioactive-emission data for a tomographic image;
 - a timing mechanism, in communication with each single-pixel detector, configured for enabling time-binning of the radioactive emissions impinging upon each single-pixel detector to time periods not greater than substantially 30 seconds; and
 - a position-tracker, configured for providing information on the position and orientation of each detecting unit, with respect to the overall structure, substantially at all times, during the individual motion,
 - the dynamic SPECT camera being configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 300 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.
2. The dynamic SPECT camera of claim 1, and further including a control unit.
3. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic

centimeters, during an acquisition time of 200 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

4. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 100 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

5. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 60 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

6. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

7. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 20 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

8. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 10 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

9. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic

centimeters, during an acquisition time of 5 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

10. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 1 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

11. The dynamic SPECT camera of claim 1, further configured for acquiring a series of tomographic reconstruction images of a region of interest of about 15 X 15 X 15 cubic centimeters, as a function of time, at a rate of at least a tomographic reconstruction image every 300 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

12. The dynamic SPECT camera of claim 1, further configured for acquiring a series of tomographic reconstruction images of a region of interest of about 15 X 15 X 15 cubic centimeters, as a function of time, at a rate of at least a tomographic reconstruction image every 200 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

13. The dynamic SPECT camera of claim 1, further configured for acquiring a series of tomographic reconstruction images of a region of interest of about 15 X 15 X 15 cubic centimeters, as a function of time, at a rate of at least a tomographic reconstruction image every 100 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

14. The dynamic SPECT camera of claim 1, further configured for acquiring a series of tomographic reconstruction images of a region of interest of about 15 X 15 X 15 cubic centimeters, as a function of time, at a rate of at least a tomographic reconstruction image every 60 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

15. The dynamic SPECT camera of claim 1, further configured for acquiring a series of tomographic reconstruction images of a region of interest of about 15 X 15 X 15 cubic centimeters, as a function of time, at a rate of at least a tomographic reconstruction image every 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

16. The dynamic SPECT camera of claim 1, further configured for acquiring a series of tomographic reconstruction images of a region of interest of about 15 X 15 X 15 cubic centimeters, as a function of time, at a rate of at least a tomographic reconstruction image every 10 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

17. The dynamic SPECT camera of claim 1, further configured for acquiring a series of tomographic reconstruction images of a region of interest of about 15 X 15 X 15 cubic centimeters, as a function of time, at a rate of at least a tomographic reconstruction image every 5 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

18. The dynamic SPECT camera of claim 1, further configured for acquiring a series of tomographic reconstruction images of a region of interest of about 15 X 15 X 15 cubic centimeters, as a function of time, at a rate of at least a tomographic reconstruction image every 1 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

19. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 7 X 7 X 7 cubic millimeter.

20. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 4 X 4 X 4 cubic millimeter.

21. The dynamic SPECT camera of claim 1, further configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 1 X 1 X 1 cubic millimeter.

22. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time stamping at an accuracy of 1 second.

23. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time stamping at an accuracy of 0.1 second.

24. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time stamping at an accuracy of 0.05 second.

25. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time stamping at an accuracy of 0.01 seconds.

26. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time stamping at an accuracy of 0.001 seconds.

27. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time binning to time bins of 1 second.

28. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time binning to time bins of 0.1 second.

29. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time binning to time bins of 0.05 second.

30. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time binning to time bins of 0.01 seconds.

31. The dynamic SPECT camera of claim 1, wherein the timing mechanism includes time binning to time bins of 0.001 seconds.

32. The dynamic SPECT camera of claim 1, and further including cardiac gating, at gated periods of substantially 50 milliseconds.

33. The dynamic SPECT camera of claim 1, employing an open collimator design, of a solid collection angle of at least 0.005 steradians, and configured for maintaining the spatial resolution, by motion in a stop and shoot acquisition mode, at very small incremental steps, of between about 0.01 degrees and about 0.75 degrees.

34. The dynamic SPECT camera of claim 1, employing an open collimator design, of a solid collection angle of at least 0.005 steradians, and configured for maintaining the spatial resolution, by a combination of:

motion in a stop and shoot acquisition mode, at very small incremental steps, of between about 0.01 degrees and about 0.75 degrees; and

simultaneous acquisition by the first plurality of the assemblies, each scanning the same region of interest from a different viewing position, thus achieving both shorter acquisition time and better edge definitions.

35. The dynamic SPECT camera of claim 1, employing an open collimator design, of a solid collection angle of at least 0.005 steradians, and configured for maintaining the spatial resolution, by a combination of:

motion in a stop and shoot acquisition mode, at very small incremental steps, of between about 0.01 degrees and about 0.75 degrees;

simultaneous acquisition by the first plurality of the assemblies, each scanning the same region of interest from a different viewing position, thus achieving both shorter acquisition time and better edge definitions; and

a structure that conforms to the body contours, for acquisition with substantial contact with the body.

36. The dynamic SPECT camera of claim 1, configured for simultaneous acquisition by the first plurality of the assemblies, each scanning the same region of interest from a different viewing position, thus achieving both shorter acquisition time and better edge definitions.

37. The dynamic SPECT camera of claim 1, wherein the individual assembly motion with respect to the overall structure is an oscillatory sweeping motion.

38. The dynamic SPECT camera of claim 37, wherein the oscillatory sweeping motion is along a longitudinal axis of the assembly.

39. The dynamic SPECT camera of claim 37, wherein the oscillatory sweeping motion is along a traverse axis of the assembly.

40. The dynamic SPECT camera of claim 37, and further including an overall array oscillatory lateral motion in at least one direction.

41. The dynamic SPECT camera of claim 37, and further including an overall array oscillatory lateral motion in at least two orthogonal directions.

42. The dynamic SPECT camera of claim 37, wherein the detecting units are grouped in blocks, and further including an individual block oscillatory sweeping motion, of the blocks in at least one of the assemblies, with respect to the assembly associated with the blocks, the individual block oscillatory sweeping motion being orthogonal to the individual assembly oscillatory sweeping motion, thus providing cross views.

43. The dynamic SPECT camera of claim 1, wherein the individual assembly motion with respect to the overall structure is an oscillatory lateral motion.

44. The dynamic SPECT camera of claim 43, wherein the oscillatory lateral motion is along a longitudinal axis of the assembly.

45. The dynamic SPECT camera of claim 43, wherein the oscillatory lateral motion is along a traverse axis of the assembly.

46. The dynamic SPECT camera of claim 1, wherein the individual assembly motion with respect to the overall structure is a combination of at least one oscillatory sweeping motion and at least one oscillatory lateral motion.

47. The dynamic SPECT camera of claim 1, wherein the assemblies in the array are configured to provide stereo views in a plane and cross views.

48. The dynamic SPECT camera of claim 1, configured for automatically receiving a precise time of radiopharmaceutical administration.

49. The dynamic SPECT camera of claim 46, wherein the administration mode is bolus administration.

50. The dynamic SPECT camera of claim 46, wherein the administration mode is slow-drip, steady state administration.

51. The dynamic SPECT camera of claim 46, wherein the administration mode is a sinusoidal administration mode.

52. The dynamic SPECT camera of claim 1, configured for continuous acquisition mode.

53. The dynamic SPECT camera of claim 1, configured for stop and shoot acquisition mode.

54. The dynamic SPECT camera of claim 52, wherein each assembly is configured for a short damping time of less than 5 second.

55. The dynamic SPECT camera of claim 52, wherein each assembly is configured for a short damping time of less than 1 second.

56. The dynamic SPECT camera of claim 52, configured for interlacing acquisition mode.

57. The dynamic SPECT camera of claim 1, configured for a combination of continuous acquisition mode and stop and shoot acquisition mode.

58. The dynamic SPECT camera of claim 1, configured for stationary prescanning.

59. The dynamic SPECT camera of claim 1, and further including an optimal electrical scheme for minimal saturation and for fast throughput.

60. The dynamic SPECT camera of claim 1, and further including active vision.

61. The dynamic SPECT camera of claim 1, and further including non-uniform voxel definition.

62. The dynamic SPECT camera of claim 1, and further including anatomic voxel definition.

63. The dynamic SPECT camera of claim 1, and further including presenting results using 5 levels of severity, from healthy to severe.

64. The dynamic SPECT camera of claim 1, configured for cardiac perfusion studies.

65. The dynamic SPECT camera of claim 1, configured for brain perfusion studies.

66. The dynamic SPECT camera of claim 1, configured for kidney perfusion studies.

67. The dynamic SPECT camera of claim 1, configured for stomach perfusion studies.

68. The dynamic SPECT camera of claim 1, configured for tumor perfusion studies.

69. The dynamic SPECT camera of claim 1, configured for acquiring a "clinically-valuable image."

70. The dynamic SPECT camera of claim 1, configured for time binning at dynamically varying time-bin lengths.

71. The dynamic SPECT camera of claim 1, configured for dynamically determining a spectral energy bin for each detecting unit.

72. The dynamic SPECT camera of claim 1, and further including employing an anatomic construction of voxels in the imaging and the reconstruction.

73. An intracorporeal dynamic SPECT camera, comprising:
an overall structure, adapted for intracorporeal insertion through a body lumen;
an assembly, arranged along a length of the overall structure, the assembly comprising:

a plurality of detecting units, each detecting unit including:

a single-pixel detector, for detecting radioactive emissions; and

a dedicated collimator, attached to the single-pixel detector, at the proximal end thereof, with respect to a region of interest, for defining a solid collection angle δ for the detecting unit; and

a motion provider, configured for providing motion with respect to the overall structure, during the acquisition of radioactive-emission data for a tomographic image;

a timing mechanism, in communication with each single-pixel detector, configured for enabling time-binning of the radioactive emissions impinging upon each single-pixel detector to time periods not greater than substantially 30 seconds; and

a position-tracker, configured for providing information on the position and orientation of each detecting unit, with respect to the overall structure, substantially at all times, during the individual motion,

the intracorporeal dynamic SPECT camera being configured for acquiring a tomographic reconstruction image of the region of interest of about 10 X 10 X 10 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

74. The intracorporeal dynamic SPECT camera of claim 73, configured for esophagus insertion, and further including cardiac gating, at gated periods of substantially 50 milliseconds.

75. The intracorporeal dynamic SPECT camera of claim 73, employing an open collimator design, of a solid collection angle of at least 0.005 steradians, and configured for maintaining the spatial resolution, by motion in a stop and shoot acquisition mode, at very small incremental steps, of between about 0.01 degrees and about 0.75 degrees.

76. The intracorporeal dynamic SPECT camera of claim 73, wherein the motion with respect to the overall structure is an assembly oscillatory sweeping motion, along a longitudinal axis of the assembly.

77. The intracorporeal dynamic SPECT camera of claim 76, and further including an assembly oscillatory lateral motion, along a longitudinal axis of the assembly.

78. The intracorporeal dynamic SPECT camera of claim 76, wherein the detecting units are grouped in blocks, and further including an individual block oscillatory sweeping motion, with respect to the assembly, the individual block oscillatory sweeping motion being orthogonal to the individual assembly oscillatory sweeping motion, thus providing cross views.

79. The intracorporeal dynamic SPECT camera of claim 73, wherein the motion with respect to the overall structure is an assembly oscillatory lateral motion, along a longitudinal axis of the assembly.

80. The intracorporeal dynamic SPECT camera of claim 73, wherein the detecting units are grouped in blocks and the motion is an individual block oscillatory sweeping motion, with respect to the assembly.

81. The intracorporeal dynamic SPECT camera of claim 73, wherein the motion with respect to the overall structure is a combination of an assembly oscillatory sweeping motion and an assembly oscillatory lateral motion.

82. The intracorporeal dynamic SPECT camera of claim 73, wherein the assembly is configured for a short damping time of less than 5 second.

83. The intracorporeal dynamic SPECT camera of claim 73, wherein the assembly is configured for a short damping time of less than 1 second.

84. The intracorporeal dynamic SPECT camera of claim 73, configured for interlacing acquisition mode.

85. The intracorporeal dynamic SPECT camera of claim 73, configured for a combination of continuous acquisition mode and stop and shoot acquisition mode.

86. The intracorporeal dynamic SPECT camera of claim 73, configured for stationary prescanning.

87. The intracorporeal dynamic SPECT camera of claim 73, configured for the prostate.

88. The intracorporeal dynamic SPECT camera of claim 73, configured for the colon.

89. The intracorporeal dynamic SPECT camera of claim 73, configured for the esophagus.

90. The intracorporeal dynamic SPECT camera of claim 73, configured for the lungs.

91. The intracorporeal dynamic SPECT camera of claim 73, configured for a woman's reproductive organs.

92. The intracorporeal dynamic SPECT camera of claim 73, configured for tumor perfusion studies.

93. The intracorporeal dynamic SPECT camera of claim 73, and further including an ultrasound transducer, for ultrasound imaging, together with the SPECT imaging.

94. A dynamic SPECT camera of short damping time, comprising

an assembly, which defines an assembly mass, M , an assembly width, W , and an assembly thickness T , the assembly comprising a plurality of detector pixels, configured for detecting radioactive emission;

a motion provider, which provides oscillatory sweeping motion to the assembly, with an axis of rotation being x_0 , wherein the assembly is configured for data acquisition in a stop and shoot acquisition mode, which comprises a series of motion steps, each followed by a stationary, data acquisition interval,

a braking mechanism, which applies a braking force F on the assembly for the stationary, data acquisition interval,

wherein the assembly and axis of rotation are designed for a damping time constant under 50 milliseconds during which vibrations amplitude subsides to under 0.25mm.

95. A stationary SPECT camera, comprising:

an overall structure, which defines proximal and distal ends with respect to a body;

a first plurality of assemblies, arranged on the overall structure, forming an array of assemblies, each assembly comprising:

a second plurality of detecting units, each detecting unit including:

a single-pixel detector, for detecting radioactive emissions; and

a dedicated collimator, attached to the single-pixel detector, at the proximal end thereof, for defining a solid collection angle δ for the detecting unit; and

an assembly motion provider, configured for providing the assembly with individual assembly motion with respect to the overall structure, prior to the acquisition of radioactive-emission data;

a position-tracker, configured for providing information on the position and orientation of each detecting unit, with respect to the overall structure, during the individual motion,

the stationary SPECT camera being configured for acquiring a tomographic reconstruction image of a region of interest while stationary, for the whole duration of the tomographic image acquisition.

96. The stationary SPECT camera of claim 95, configured for acquiring a tomographic image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 10 minutes, at a spatial resolution of at least 20 X 20 X 20 cubic millimeter.

97. The stationary SPECT camera of claim 95, configured for acquiring a tomographic image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 5 minutes, at a spatial resolution of at least 20 X 20 X 20 cubic millimeter.

98. The stationary SPECT camera of claim 95, configured for acquiring a tomographic image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 20 X 20 X 20 cubic millimeter.

99. The stationary SPECT camera of claim 95, configured for acquiring a tomographic image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 60 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

100. The stationary SPECT camera of claim 95, configured for acquiring a tomographic image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

101. The stationary SPECT camera of claim 95, and further including a timing mechanism, in communication with each single-pixel detector, configured for enabling time-binning of the radioactive emissions impinging upon each single-pixel detector to time periods not greater than substantially 1 seconds.

102. The stationary SPECT camera of claim 95, wherein the structure conforms to the body contours, for acquisition for acquisition with substantial contact with the body.

103. The stationary SPECT camera of claim 95, wherein the assemblies in the array are configured to provide stereo views in a plane and cross views.

104. A dynamic SPECT camera, configured for time binning at dynamically varying time-bin lengths, the camera comprising:

- an overall structure, which defines proximal and distal ends with respect to a body;

- a detecting unit, arranged on the overall structure and configured for detecting radioactive emissions from the body;

- a timing mechanism, in communication with the detecting unit, configured for enabling time-binning of the radioactive emissions impinging upon the detecting unit, to time bins of the dynamically varying time-bin lengths;

- a lookup system of recommended time-bin lengths, as functions of at least one of a specific region of interest, an administered radiopharmaceutical, time since the administration of the radiopharmaceutical, cardiac state with respect to an RR cycle, a view of the detecting unit with respect to the region of interest, and data acquisition mode,

wherein the timing mechanism is configured for selecting a recommended time-bin length from the lookup system, for each time bin, for each single-pixel detector.

105. The dynamic SPECT camera of claim 104, and further including:

- a first plurality of assemblies, arranged on the overall structure, forming an array of assemblies, each assembly comprising:

- a second plurality of the detecting units, each of the detecting units including:

- a single-pixel detector, for detecting radioactive emissions; and

a dedicated collimator, attached to the single-pixel detector, at the proximal end thereof, for defining a solid collection angle δ for the detecting unit; and

an assembly motion provider, configured for providing the assembly with individual assembly motion with respect to the overall structure, during the acquisition of radioactive-emission data for a tomographic image.

106. A dynamic SPECT camera configured for dynamically determining a spectral energy bin for each detecting unit, the camera comprising:

an overall structure, which defines proximal and distal ends with respect to a body;

a plurality of detecting unit; arranged on the overall structure and configured for detecting radioactive emissions in a spectral range between 10 KeV and 1 MeV;

a spectral selection mechanism, for enabling a selection of a spectral energy bin to be used for each detecting unit, independently from the other detecting units; and

a lookup system of recommended spectral energy bin values, as functions of at least one of a specific region of interest, an administered radiopharmaceutical, time since the administration of the radiopharmaceutical, a view of the detecting unit with respect to the region of interest, and patient's details;

wherein the spectral selection mechanism is further configured for dynamically determining the spectral energy bin for each detecting unit, as functions of the specific region of interest, the administered radiopharmaceutical, the time elapsed since the administration of the radiopharmaceutical, the view of the detecting unit with respect to the region of interest, and patients' details, from the lookup system.

107. The dynamic SPECT camera of claim 106, wherein the spectral energy bin is designed to include a primary photon energy $\pm 10\%$.

108. The dynamic SPECT camera of claim 106, wherein the spectral energy bin is designed to include a primary photon energy $\pm 7\%$.

109. The dynamic SPECT camera of claim 106, wherein the spectral energy bin is designed to include a primary photon energy $\pm 5\%$.

110. The dynamic SPECT camera of claim 106, and further including administering at least two radiopharmaceuticals and viewing a same region with different groups of detecting units, each group being configured for a different spectral energy bin, so as to view each radiopharmaceutical in the same region independently of the other.

111. The dynamic SPECT camera of claim 106, wherein the spectral selection mechanism is a hardware unit.

112. The dynamic SPECT camera of claim 106, wherein the spectral selection mechanism is a software.

113. The dynamic SPECT camera of claim 106, wherein the spectral selection is performed during data acquisition.

114. The dynamic SPECT camera of claim 106, wherein the spectral selection is performed after data acquisition.

115. The dynamic SPECT camera of claim 106, and further including:
a first plurality of assemblies, arranged on the overall structure, forming an array of assemblies, each assembly comprising:

a second plurality of the detecting units, each of the detecting units including:

a single-pixel detector, for detecting radioactive emissions; and
a dedicated collimator, attached to the single-pixel detector, at the proximal end thereof, for defining a solid collection angle δ for the detecting unit; and
an assembly motion provider, configured for providing the assembly with individual assembly motion with respect to the overall structure, during the acquisition of radioactive-emission data for a tomographic image.

116. The dynamic SPECT camera of claim 106, and further including a timing mechanism.

117. A method for anatomic construction of voxels, comprising:
providing a structural image of a region of interest;
constructing an anatomic system of voxels, for the region of interest, in which voxel boundaries are aligned with boundaries of structural objects of the region of interest, based on the structural image;
performing radioactive-emission imaging of the region of interest, utilizing the anatomic system of voxels; and
performing reconstruction of the radioactive-emission imaging, utilizing the anatomic system of voxels.

118. The method of claim 117, wherein the structural image is provided by a structural imager, selected from the group consisting of 2-D ultrasound, 3-D ultrasound, planner x-rays, CT x-rays, and MRI.

119. The method of claim 118, wherein the structural imager is co-registered to a radioactive-emission imaging camera which performs the radioactive-emission imaging.

120. The method of claim 118, wherein the structural imager is not co-registered to a radioactive-emission imaging camera which performs the radioactive-emission imaging, and further including corrections for misregistration.

121. The method of claim 119, and further including attenuation correction of the radioactive-emission imaging based on the structural image.

122. The method of claim 119, and further including displaying the structural image and the reconstruction of the radioactive-emission imaging together.

123. The method of claim 117, wherein the structural image is provided from a lookup system.

124. The method of claim 123, wherein the lookup system is corrected for patient's details.

125. The method of claim 117, and further including fitting the boundaries of the structural objects to parametric equations and utilizing the parametric equations in the constructing of the anatomic system of voxels.

126. The method of claim 117, wherein the anatomic system of voxels includes voxels of varying volumes, depending on their anatomic position and relevance.

127. The method of claim 117, and further including time-binning of the radioactive emissions to time periods not greater than substantially 30 seconds,

128. The method of claim 127, wherein the anatomic system of voxels includes voxels of varying volumes, depending on the relevance of their dynamic activity.

129. A method of reconstruction of a radioactive emission image, comprising:
providing a first system of voxels for a region of interest;
obtaining radioactive-emission data from the region of interest;
performing a first reconstruction, based on the radioactive-emission data and the first system of voxels, to obtain a first image;
correcting the first system of voxels, by aligning voxel boundaries with object boundaries, based on the first image; thus obtaining a second system of voxels;
performing a second reconstruction, based on the radioactive-emission data and the second system of voxels, thus obtaining a second image.

130. A method of reconstruction of a radioactive emission image, comprising:
providing a first system of voxels for a region of interest;

obtaining a first set of radioactive-emission data from the region of interest;
performing a first reconstruction, based on the first set of the radioactive-emission data and the first system of voxels, to obtain a first image;
correcting the first system of voxels, by aligning voxel boundaries with object boundaries, based on the first image; thus obtaining a second system of voxels;
obtaining a second set of radioactive-emission data from the region of interest, based on the second system of voxels; and
performing a second reconstruction, based on the second set of the radioactive-emission data and the second system of voxels, thus obtaining a second image.

131. A method of dynamic SPECT data acquisition, comprising:

providing a timing mechanism, in communication with each single-pixel detector for enabling time-binning of radioactive emissions impinging upon each single-pixel detector of a SPECT camera to time periods not greater than substantially 30 seconds; and

providing information on the position and orientation of each single-pixel detector of the SPECT camera, with respect to the overall structure, substantially at all times, during the image acquisition; and

acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter.

132. A method of time binning SPECT data at dynamically varying time-bin lengths, the camera comprising:

providing a timing mechanism, in communication with each single-pixel detector for enabling time-binning of radioactive emissions impinging upon the single-pixel detector, to time bins of the dynamically varying time-bin lengths;

providing a lookup system of recommended time-bin lengths, as functions of at least one of a specific region of interest, an administered radiopharmaceutical, time since the administration of the radiopharmaceutical, cardiac state with respect to an RR cycle, a

view of the single-pixel detector with respect to the region of interest, and data acquisition mode,

selecting a recommended time-bin length from the lookup system, for each time bin, for each single-pixel detector.

133. A method of dynamically determining a spectral energy bin for each single-pixel detector, comprising:

providing a spectral selection mechanism, for enabling a selection of a spectral energy bin to be used for each single-pixel detector, independently from other single-pixel detectors of a SPECT camera; and

providing a lookup system of recommended spectral energy bin values, as functions of at least one of a specific region of interest, an administered radiopharmaceutical, time since the administration of the radiopharmaceutical, a view of the single-pixel detector with respect to the region of interest, and patient's details;

wherein the spectral selection mechanism is further configured for dynamically determining the spectral energy bin for each single-pixel detector, as functions of the specific region of interest, the administered radiopharmaceutical, the time elapsed since the administration of the radiopharmaceutical, the view of the single-pixel detector with respect to the region of interest, and patients' details, from the lookup system.

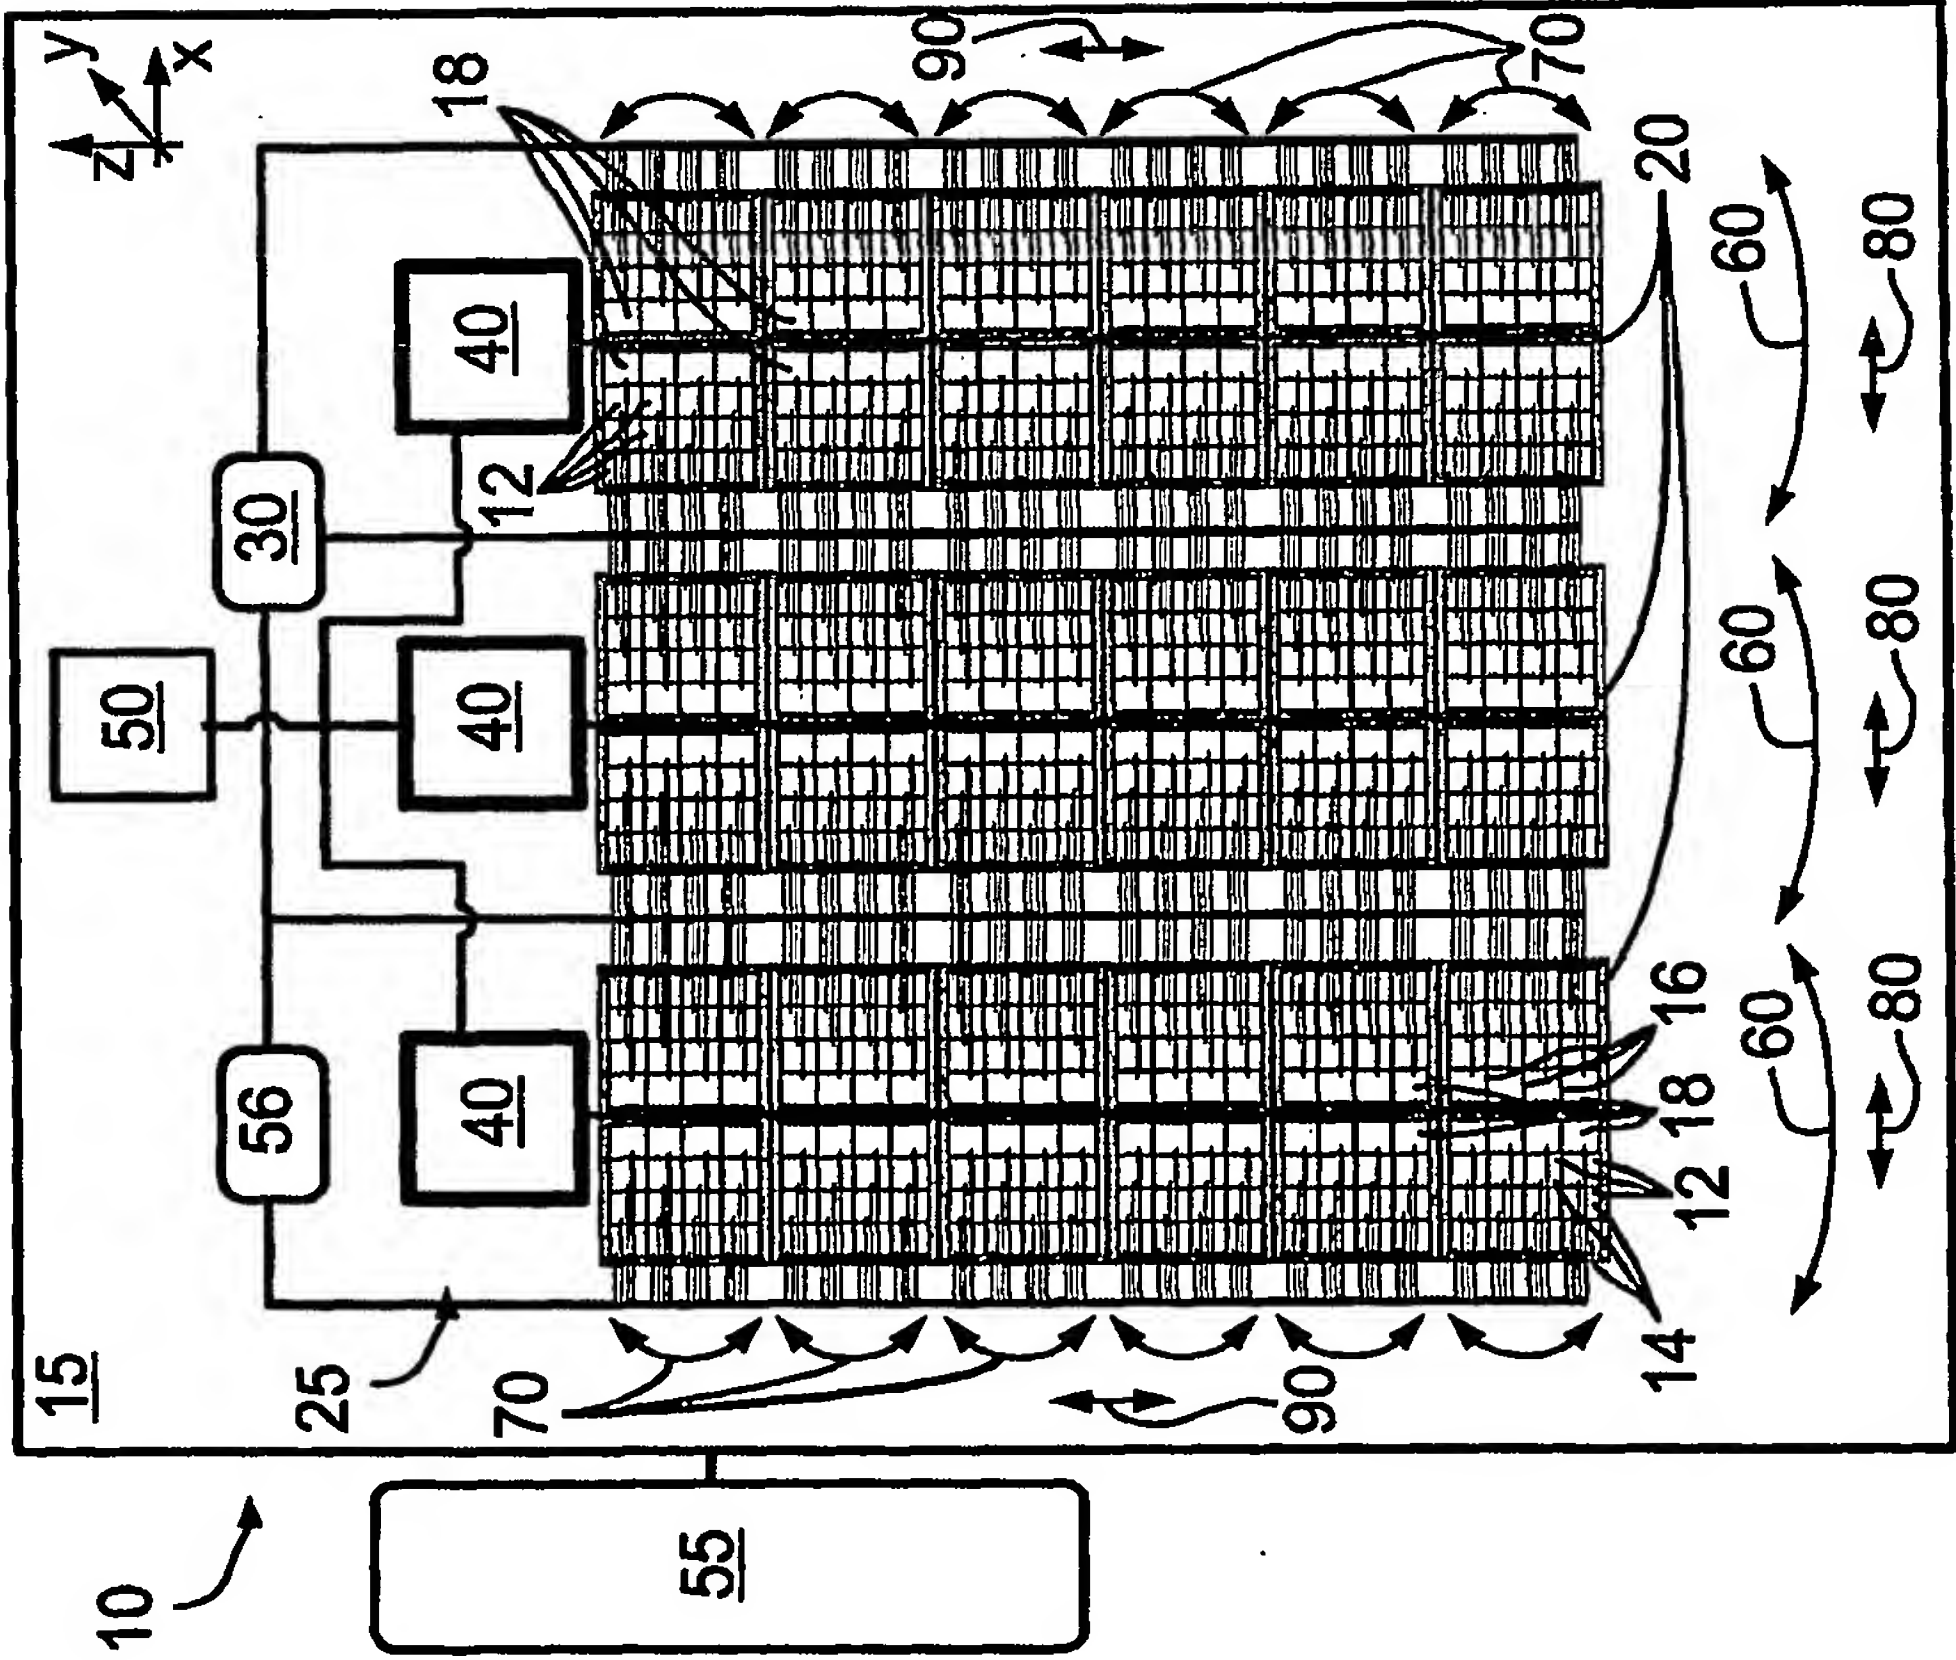


Figure 1A

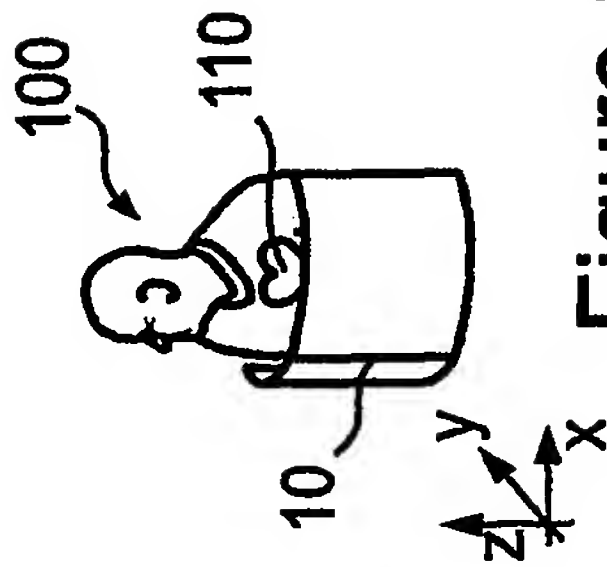


Figure 1B

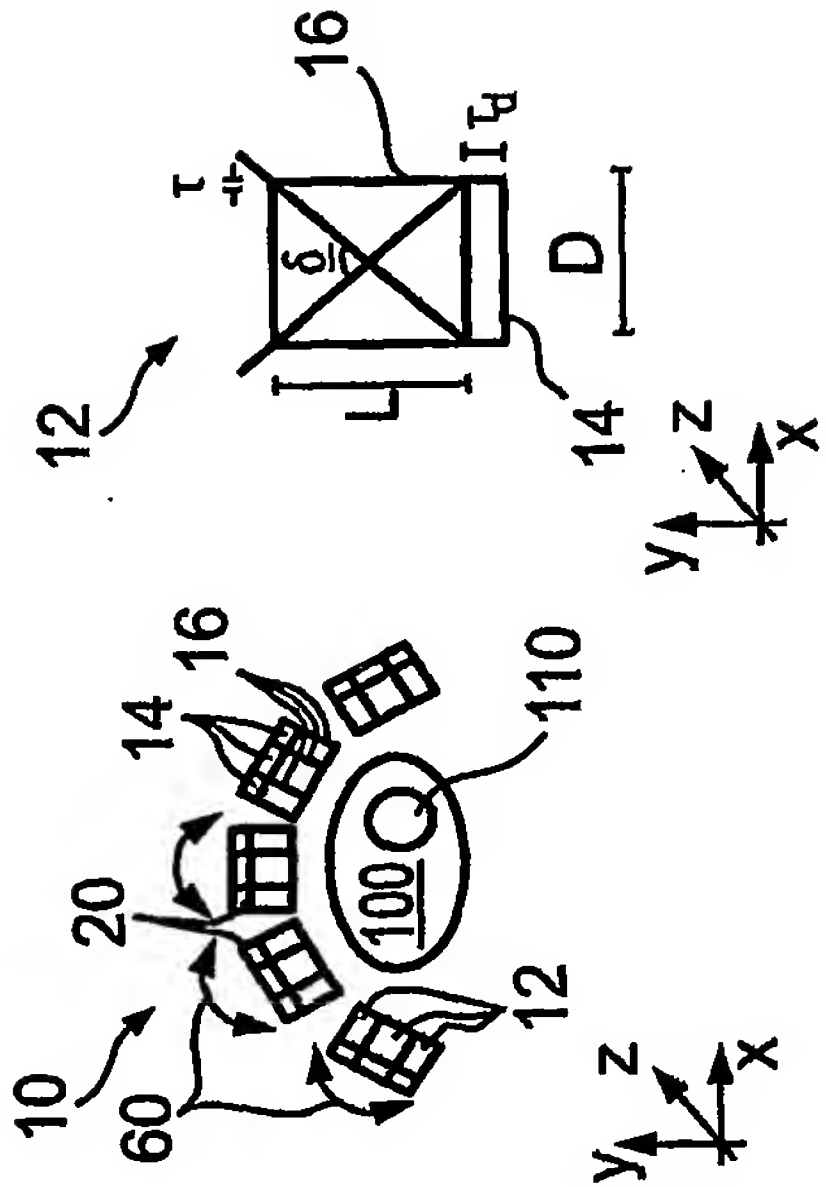
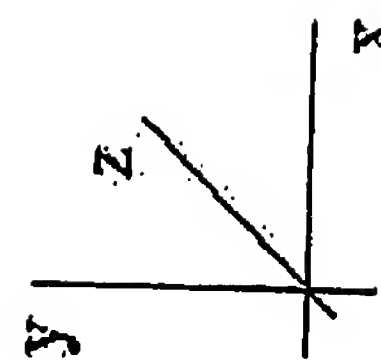
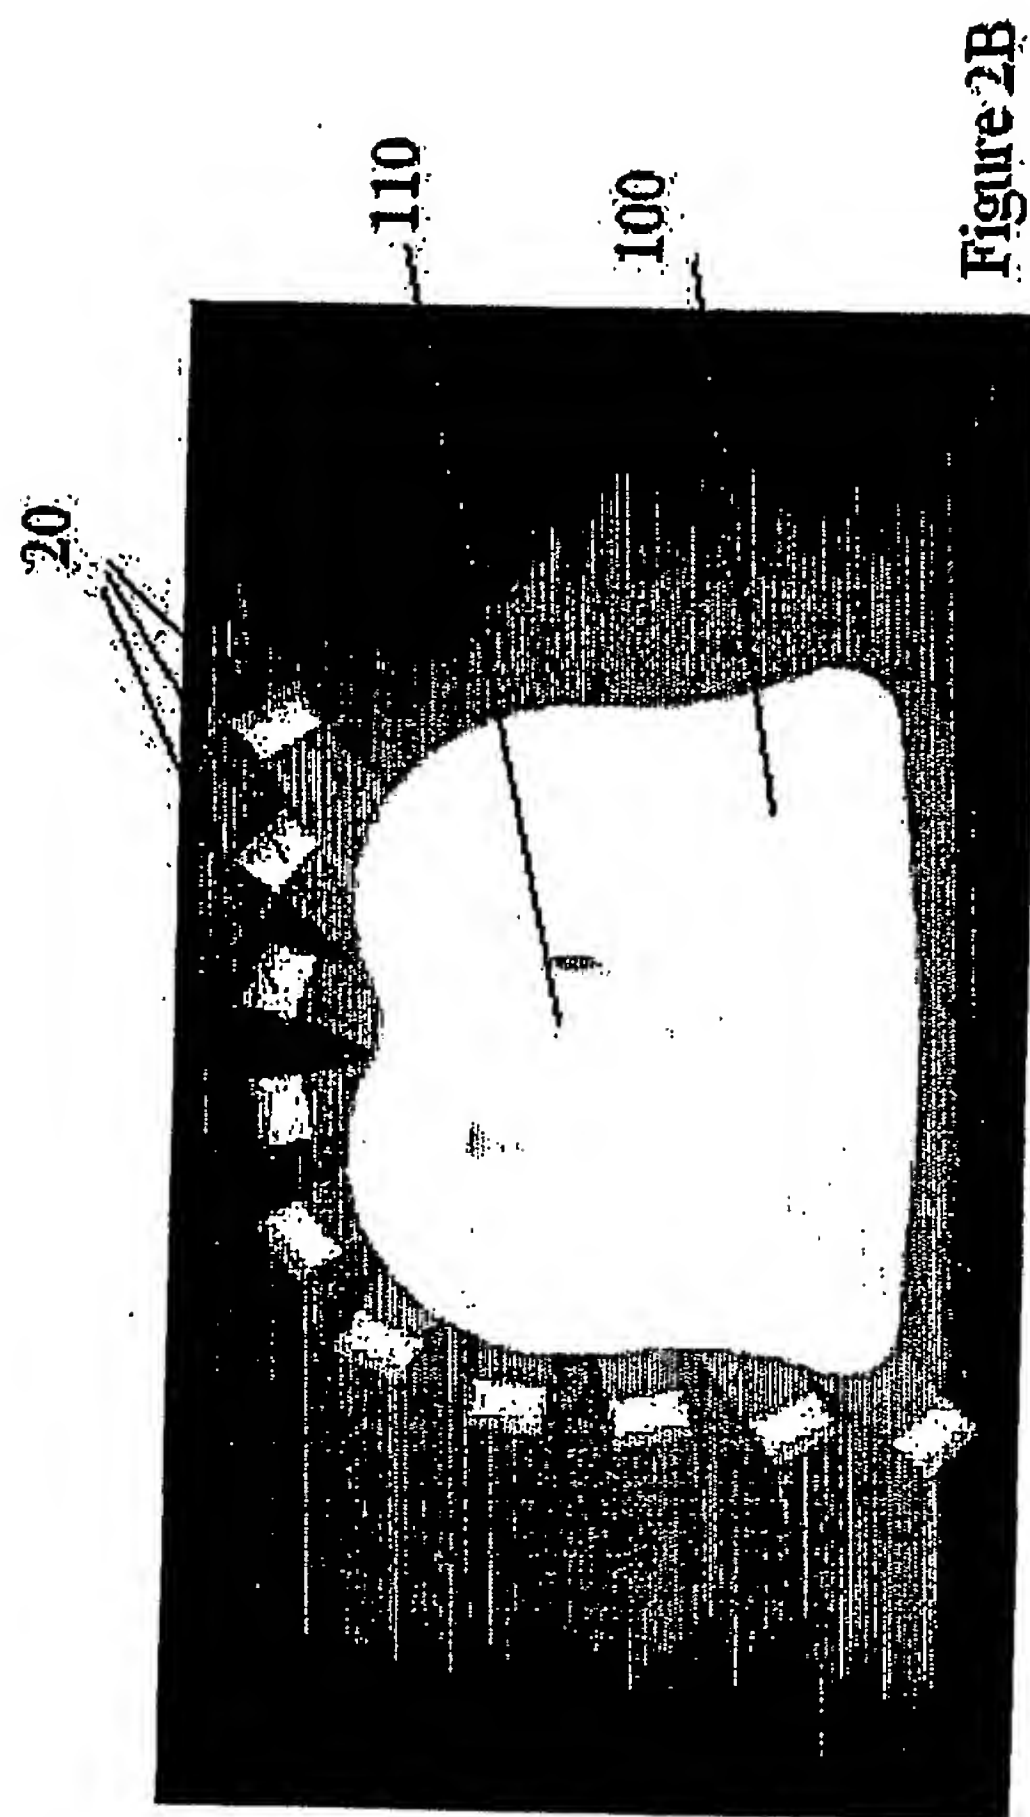
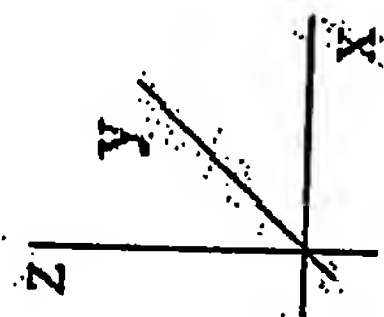
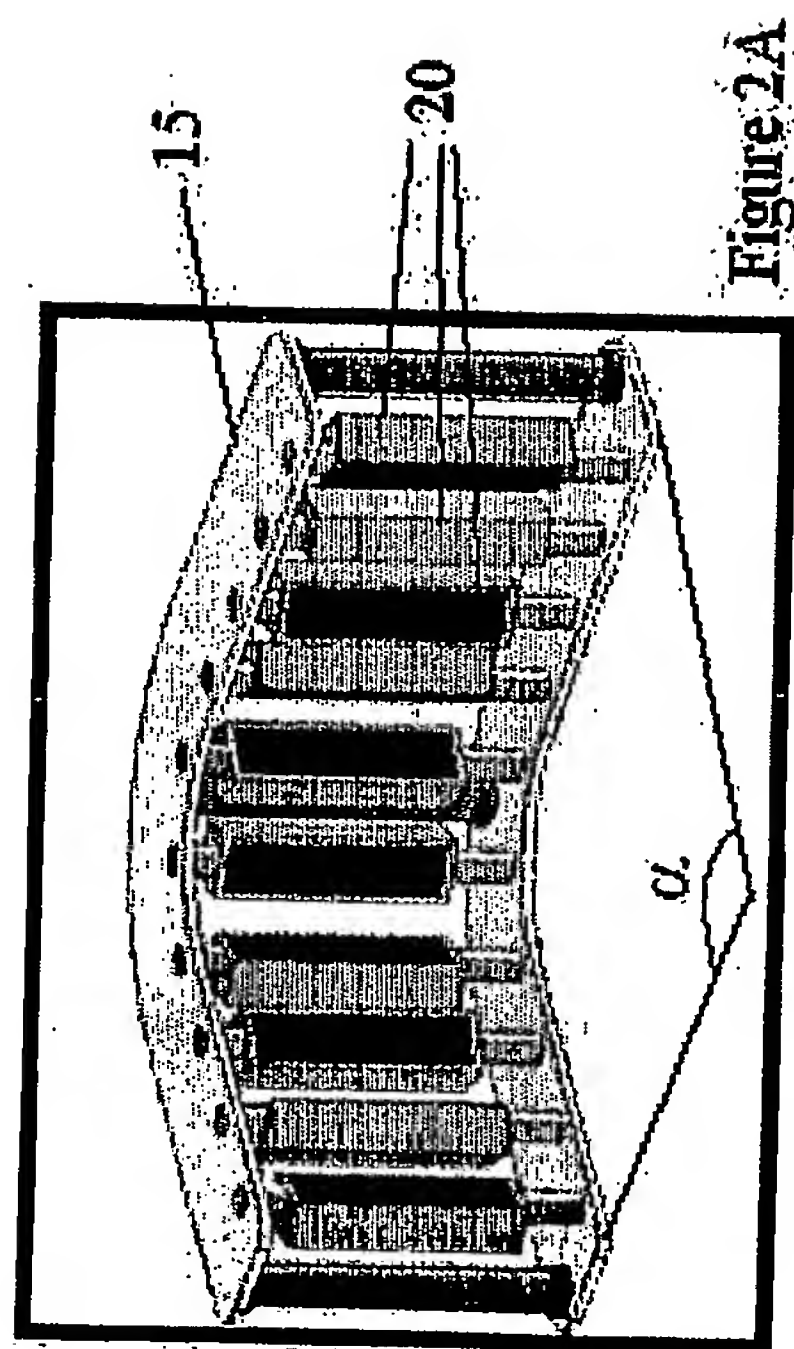


Figure 1C

Figure 1D



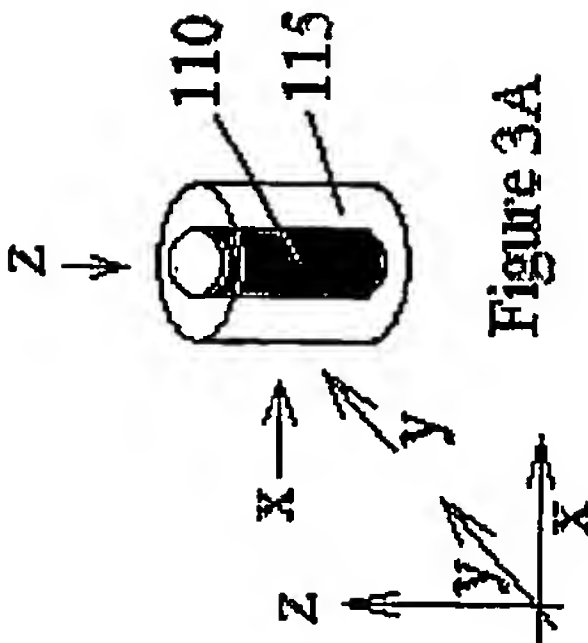


Figure 3A

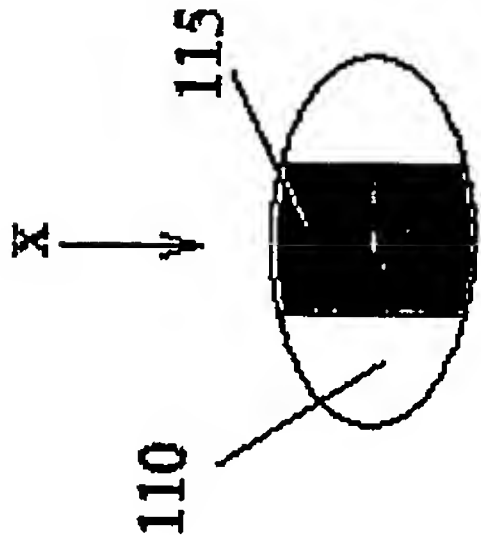


Figure 3B

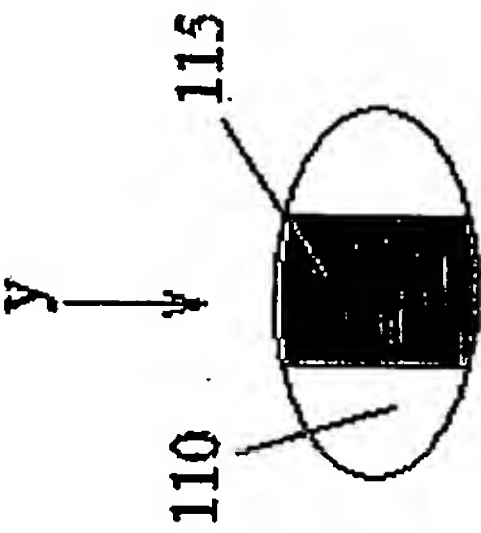


Figure 3C

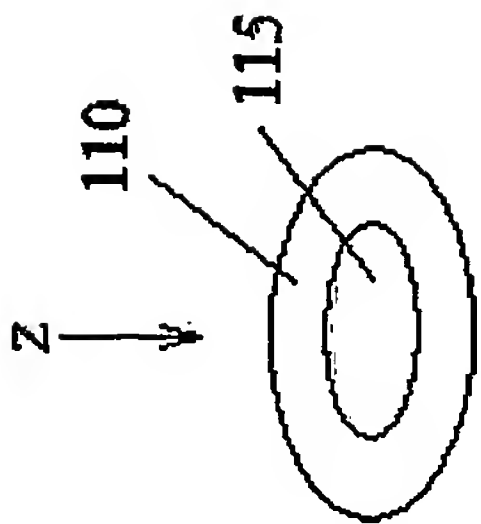
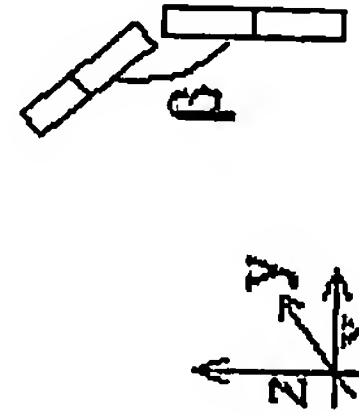
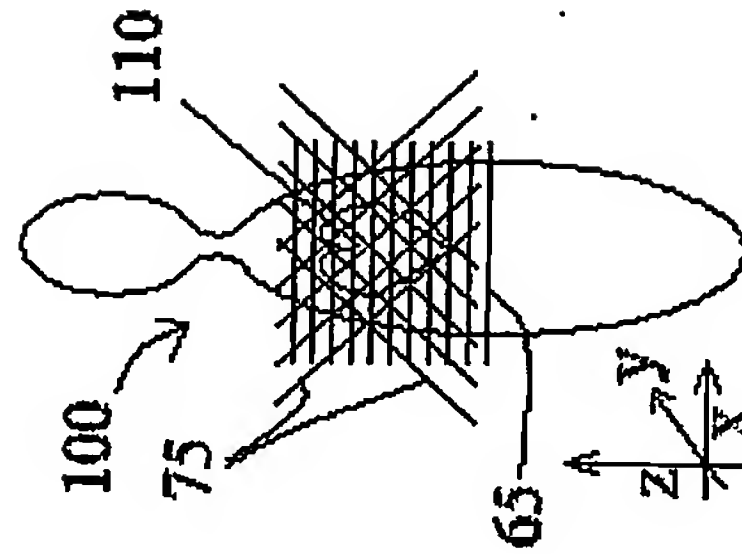
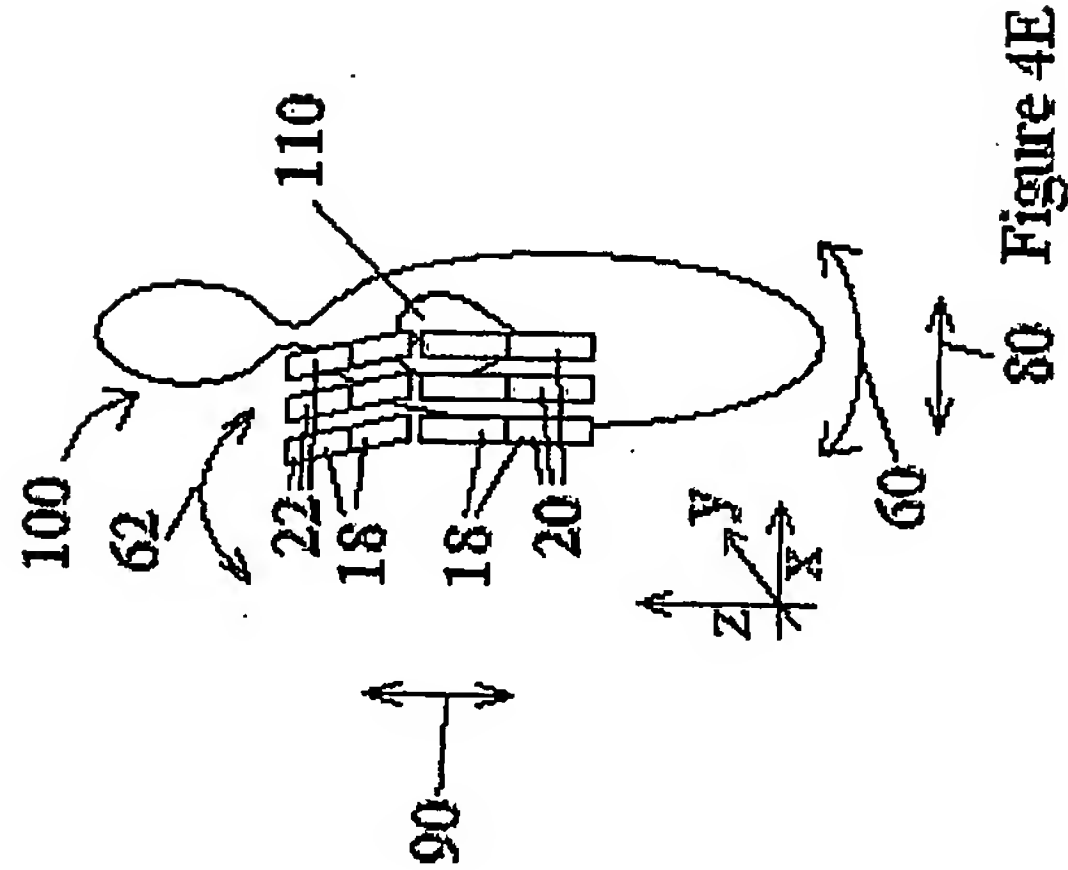
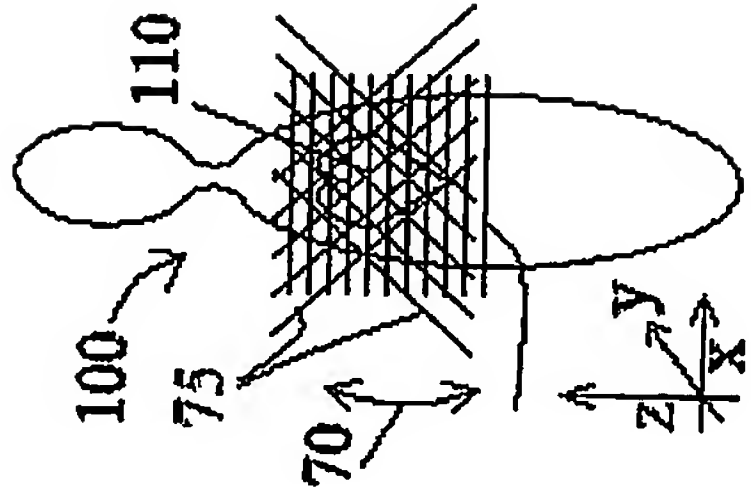
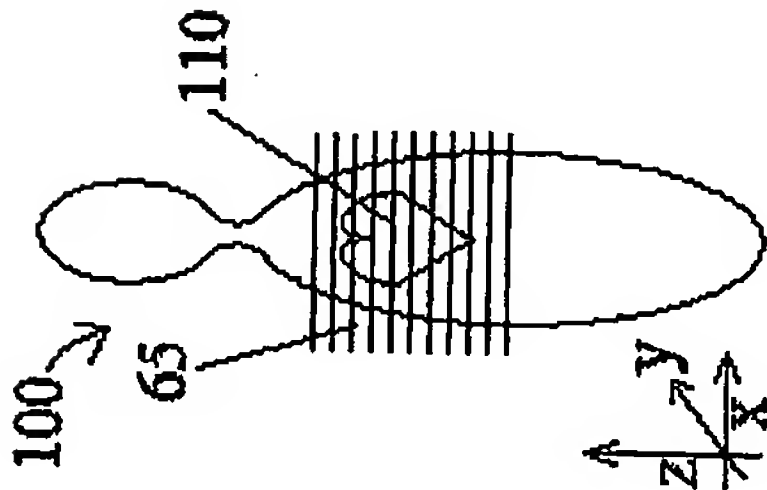
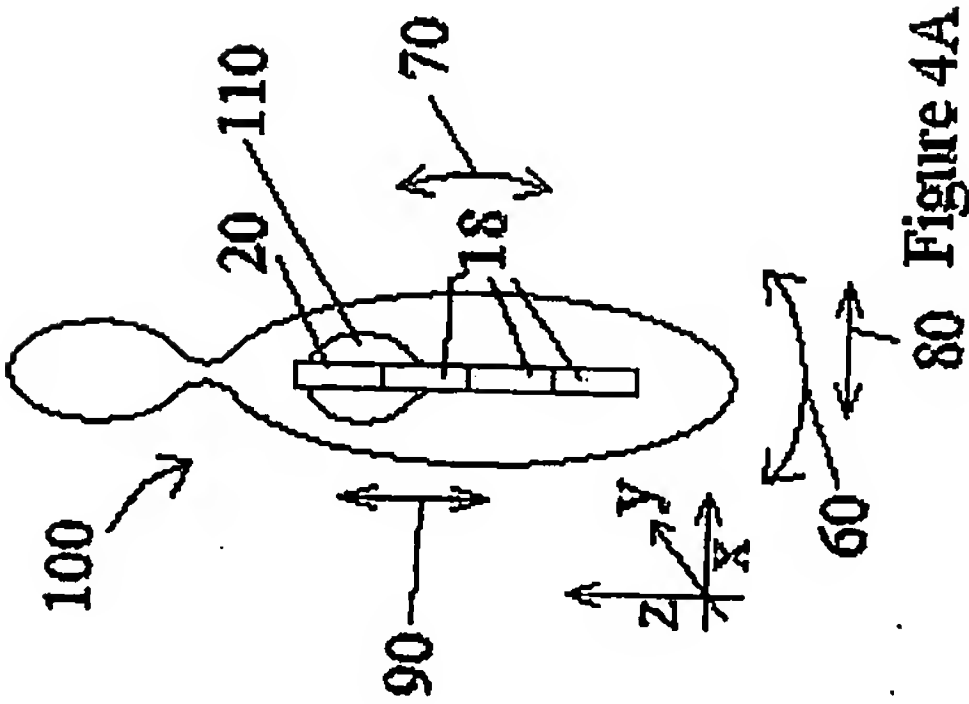


Figure 3D



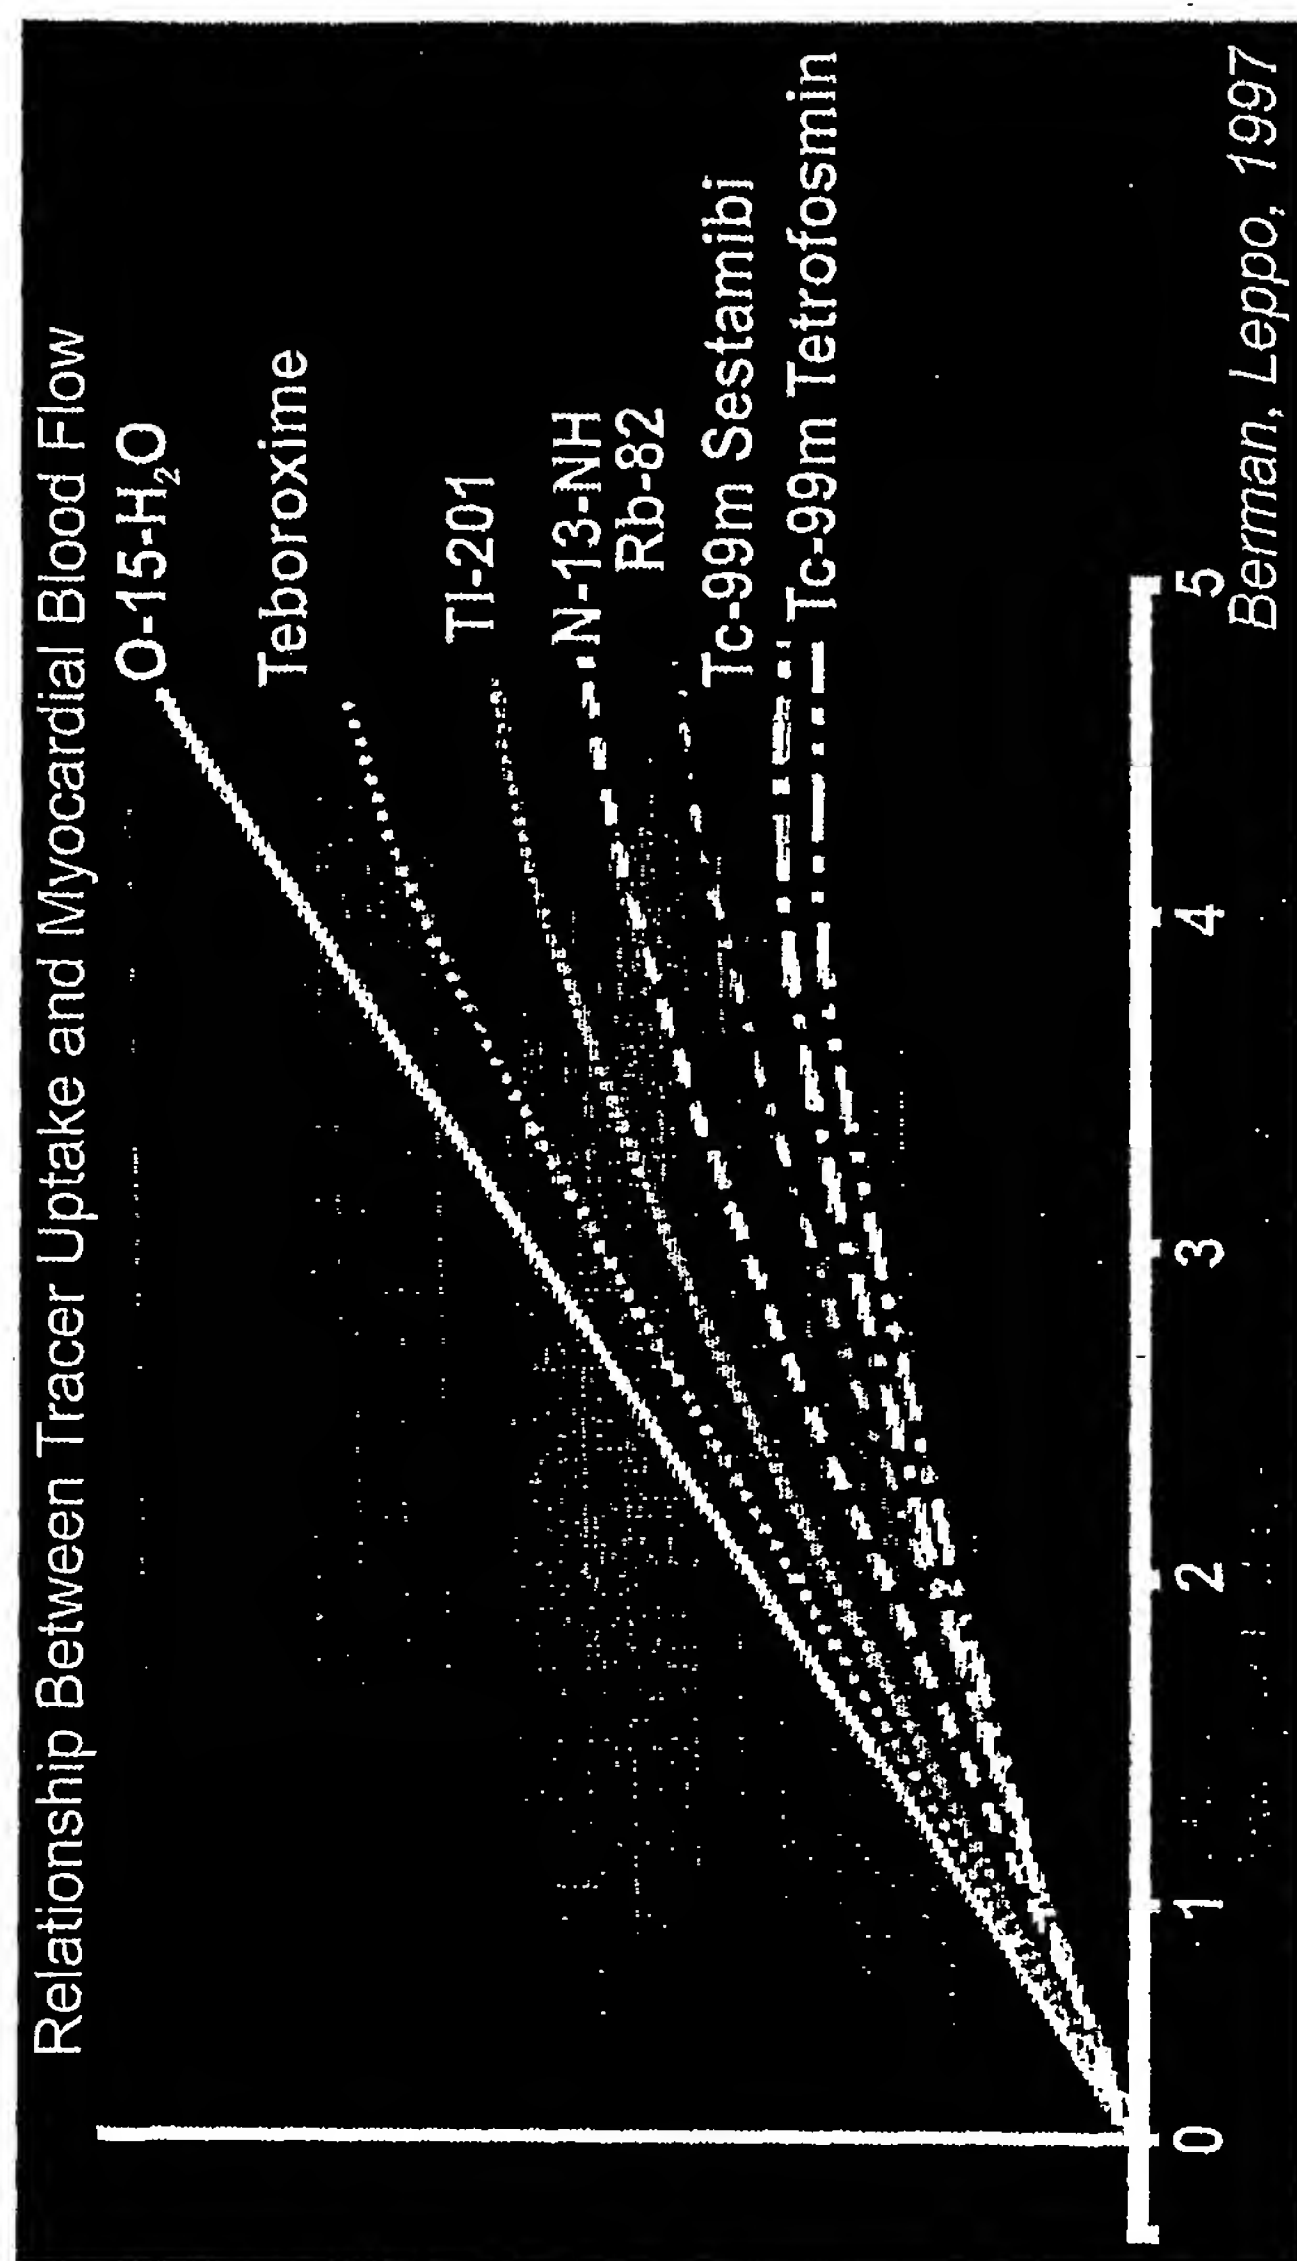


Figure 5A

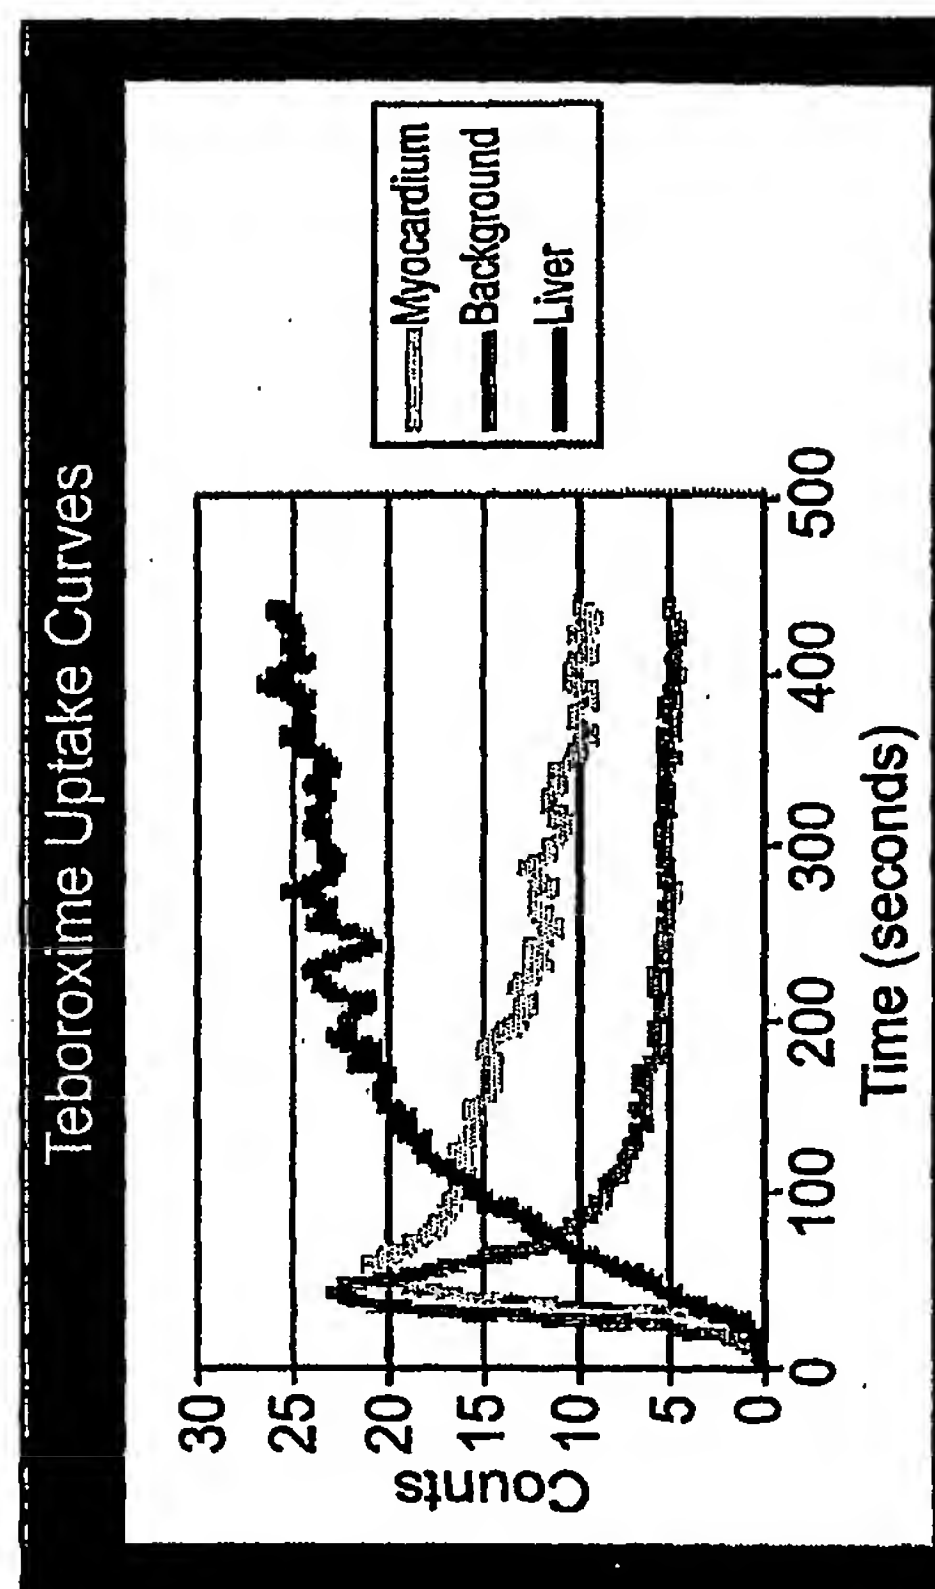
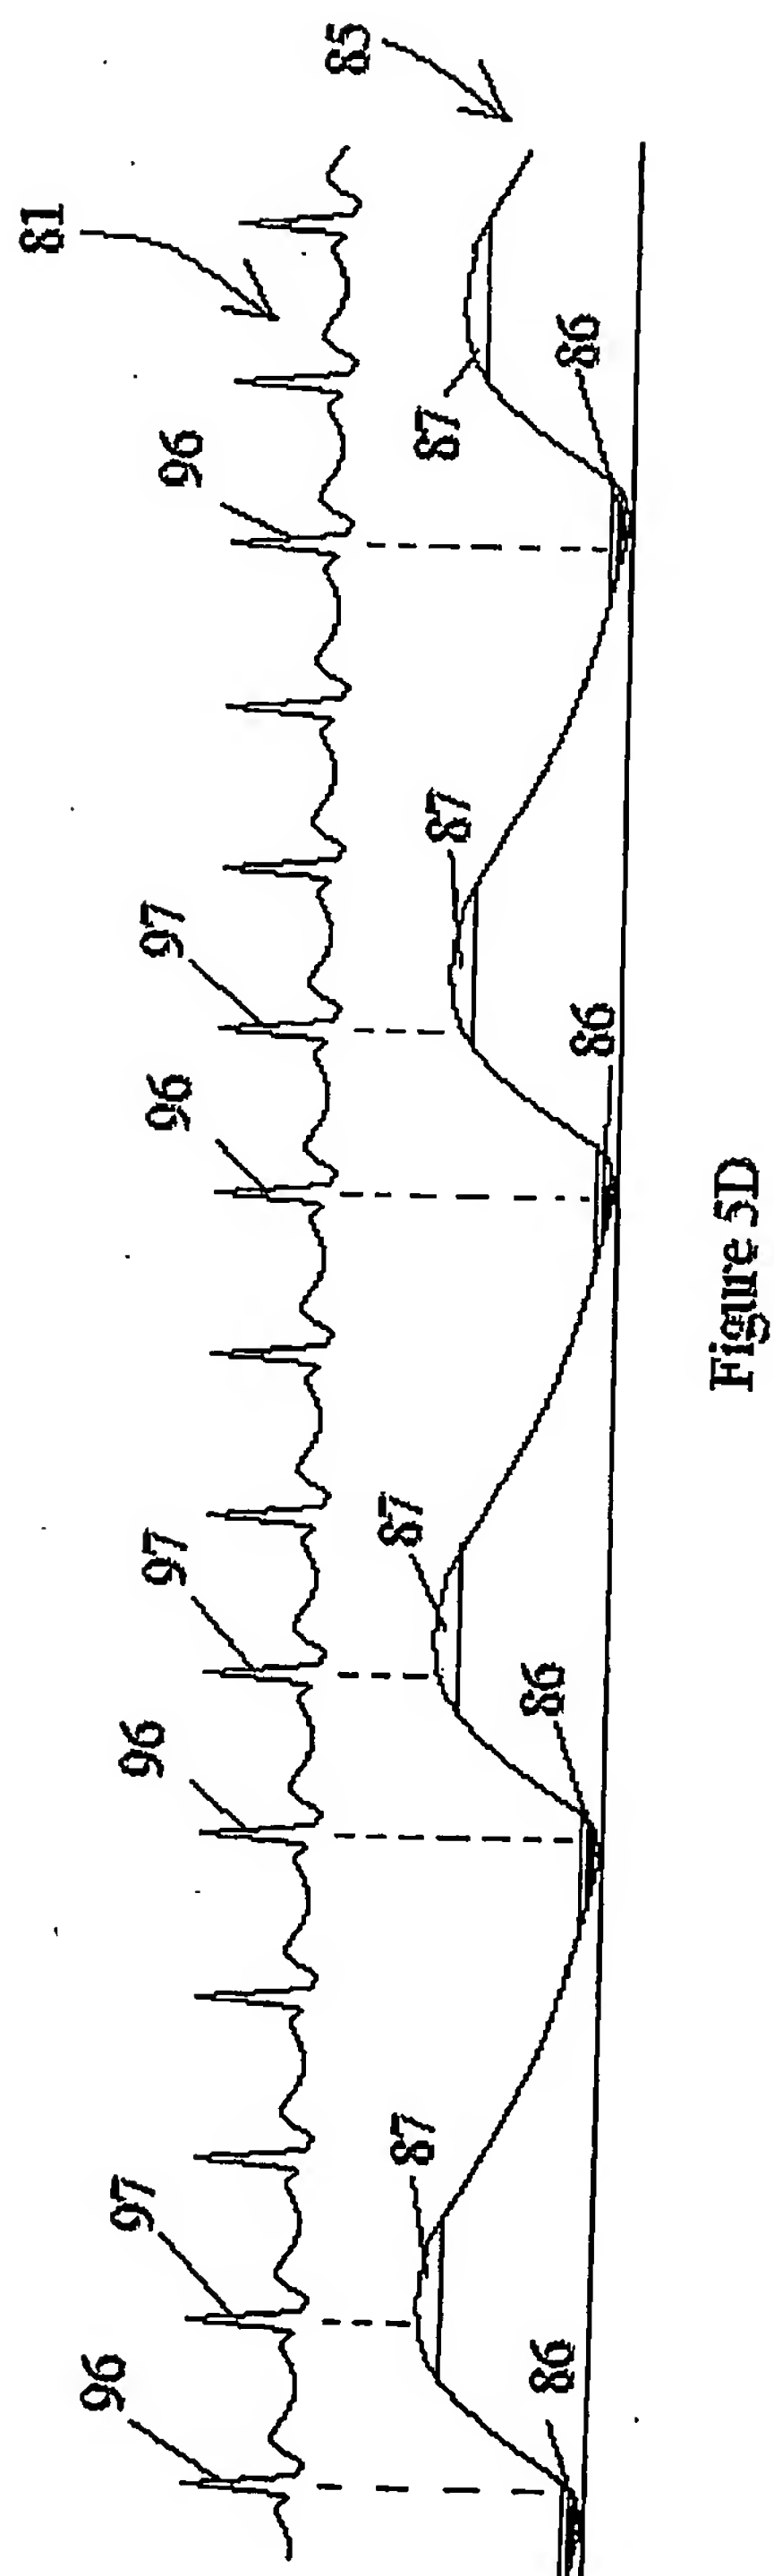
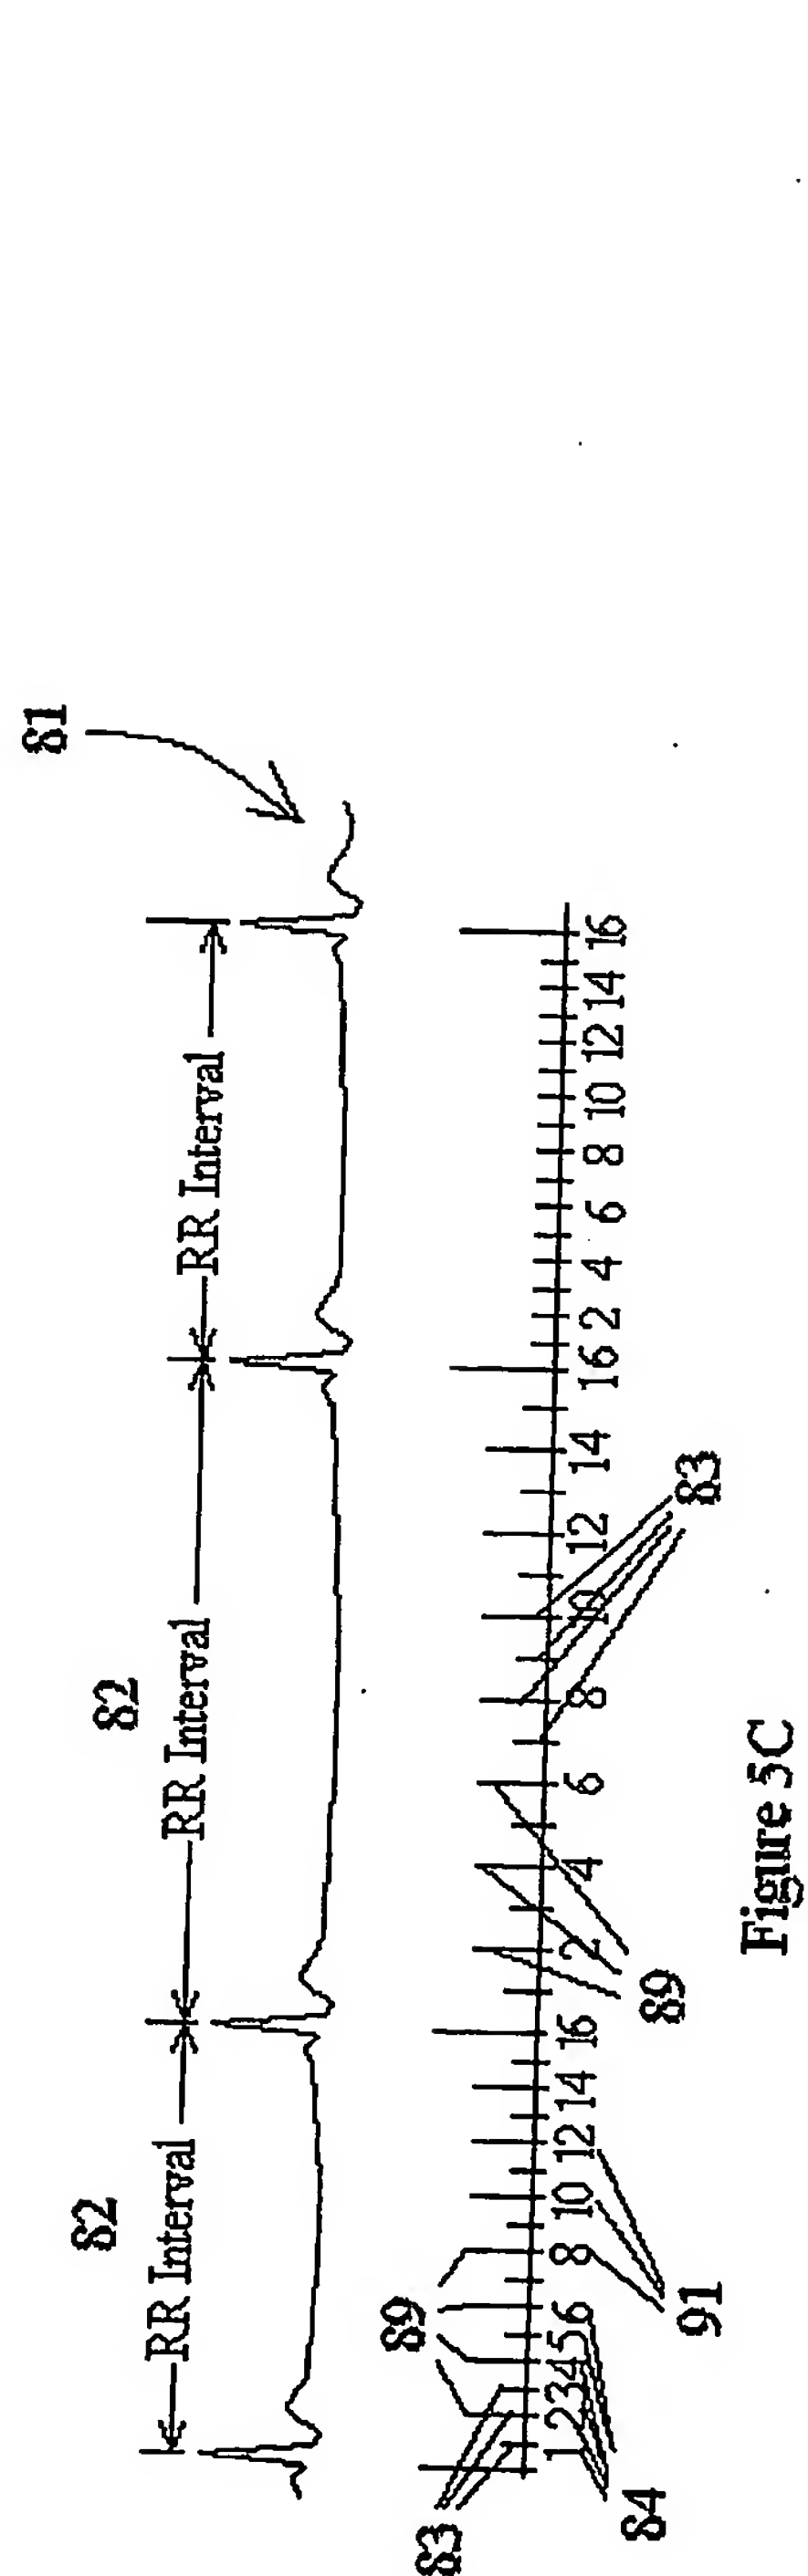


Figure 5B



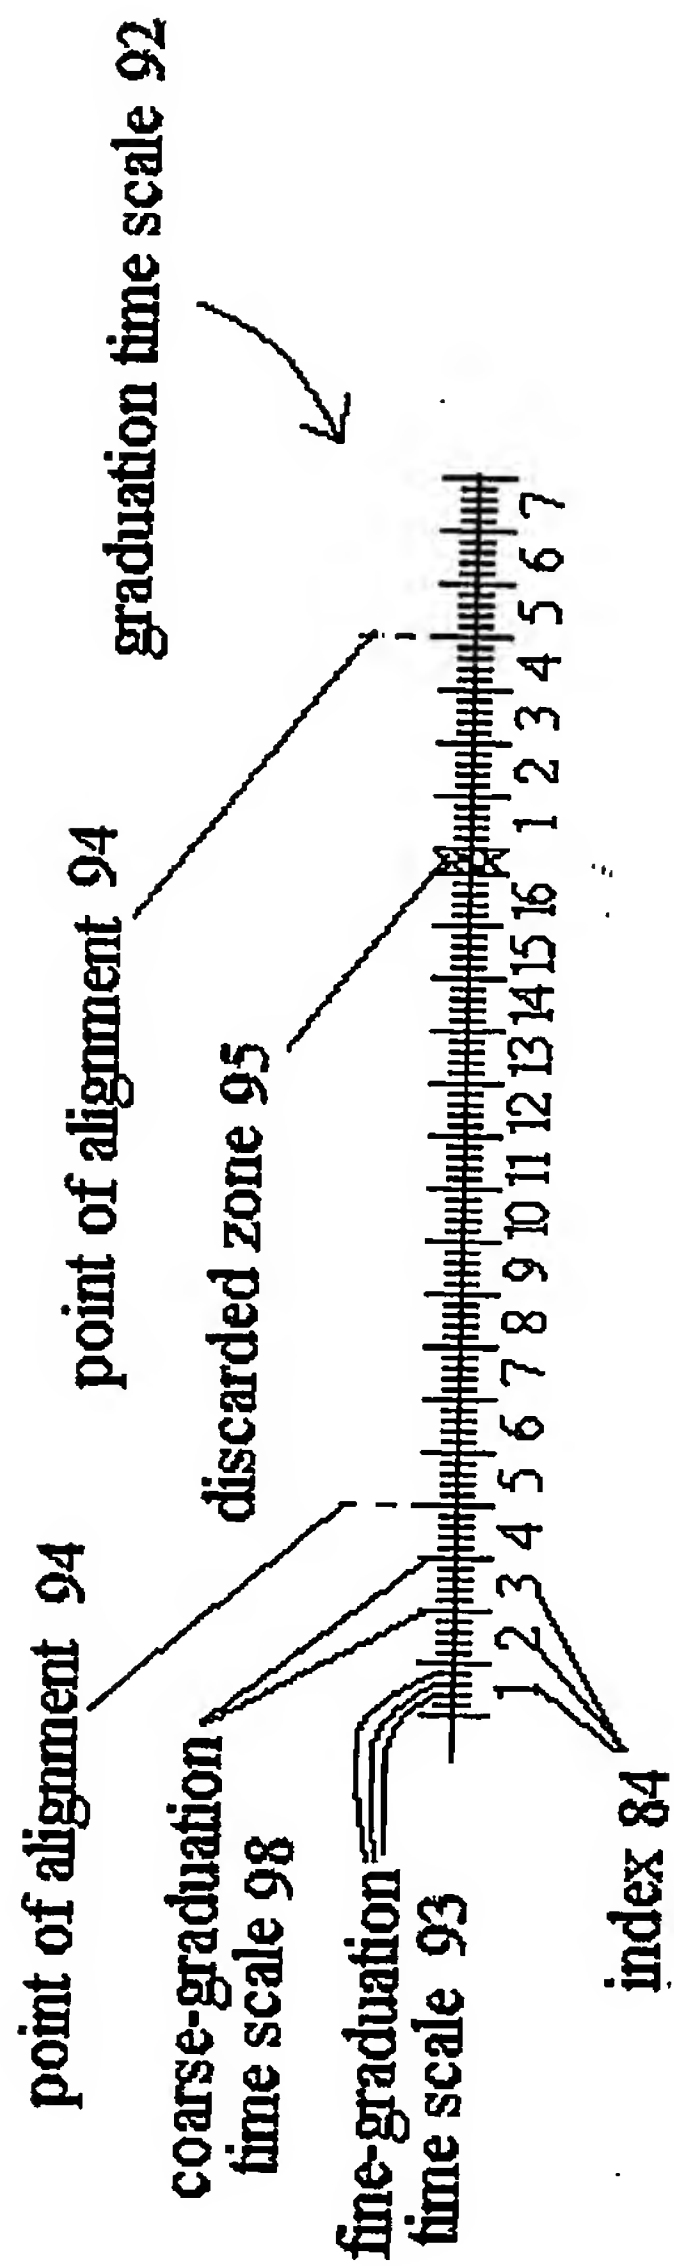


Figure 5E

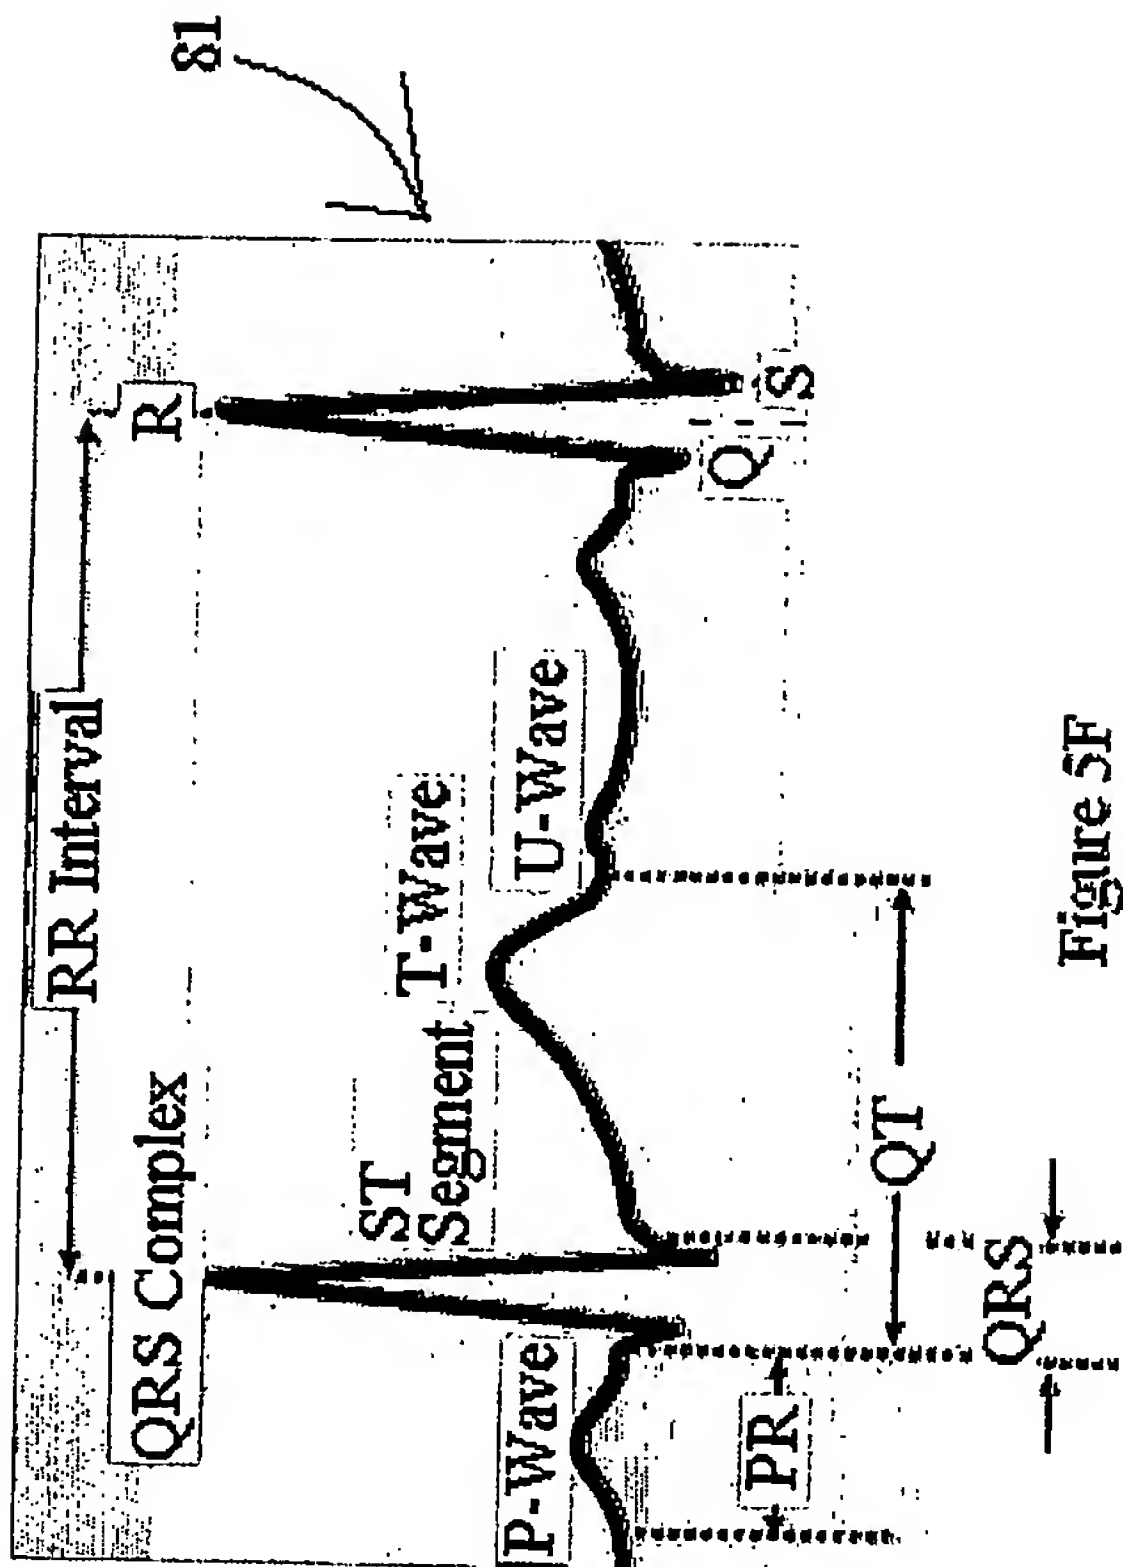


Figure 5F

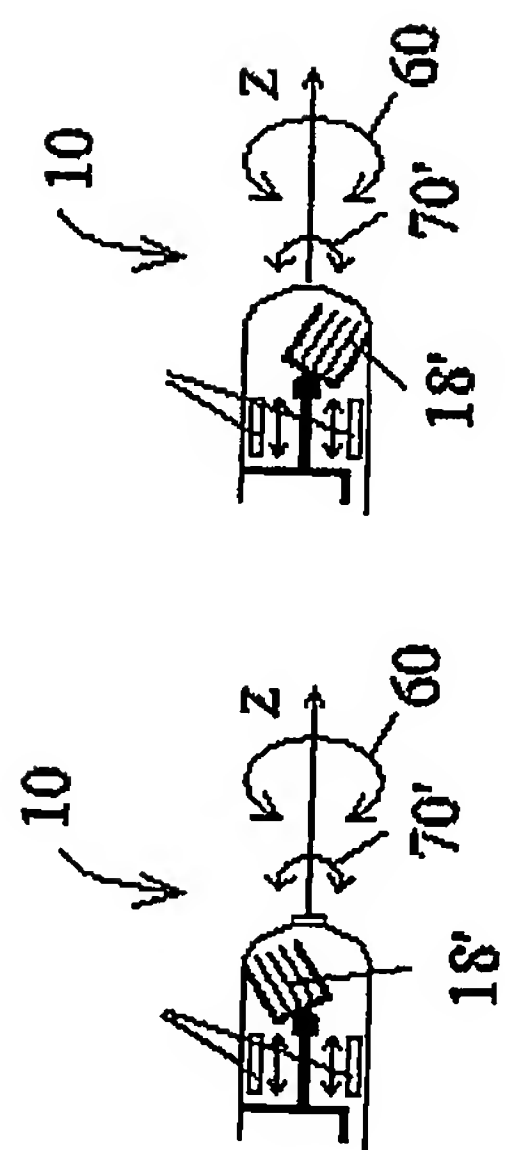
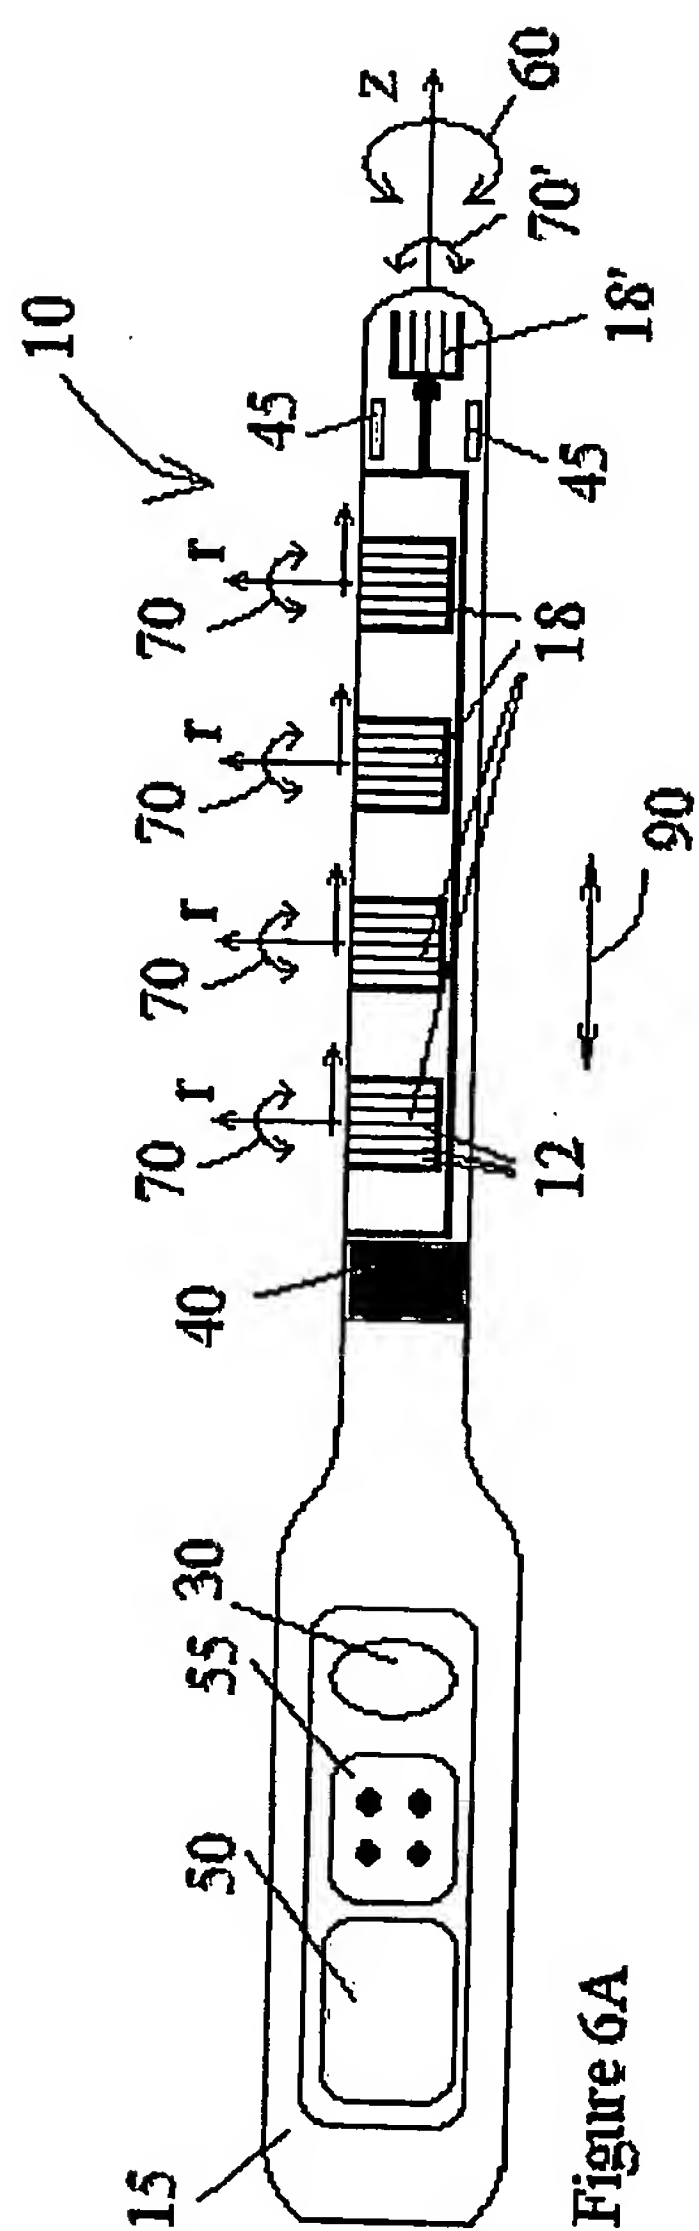
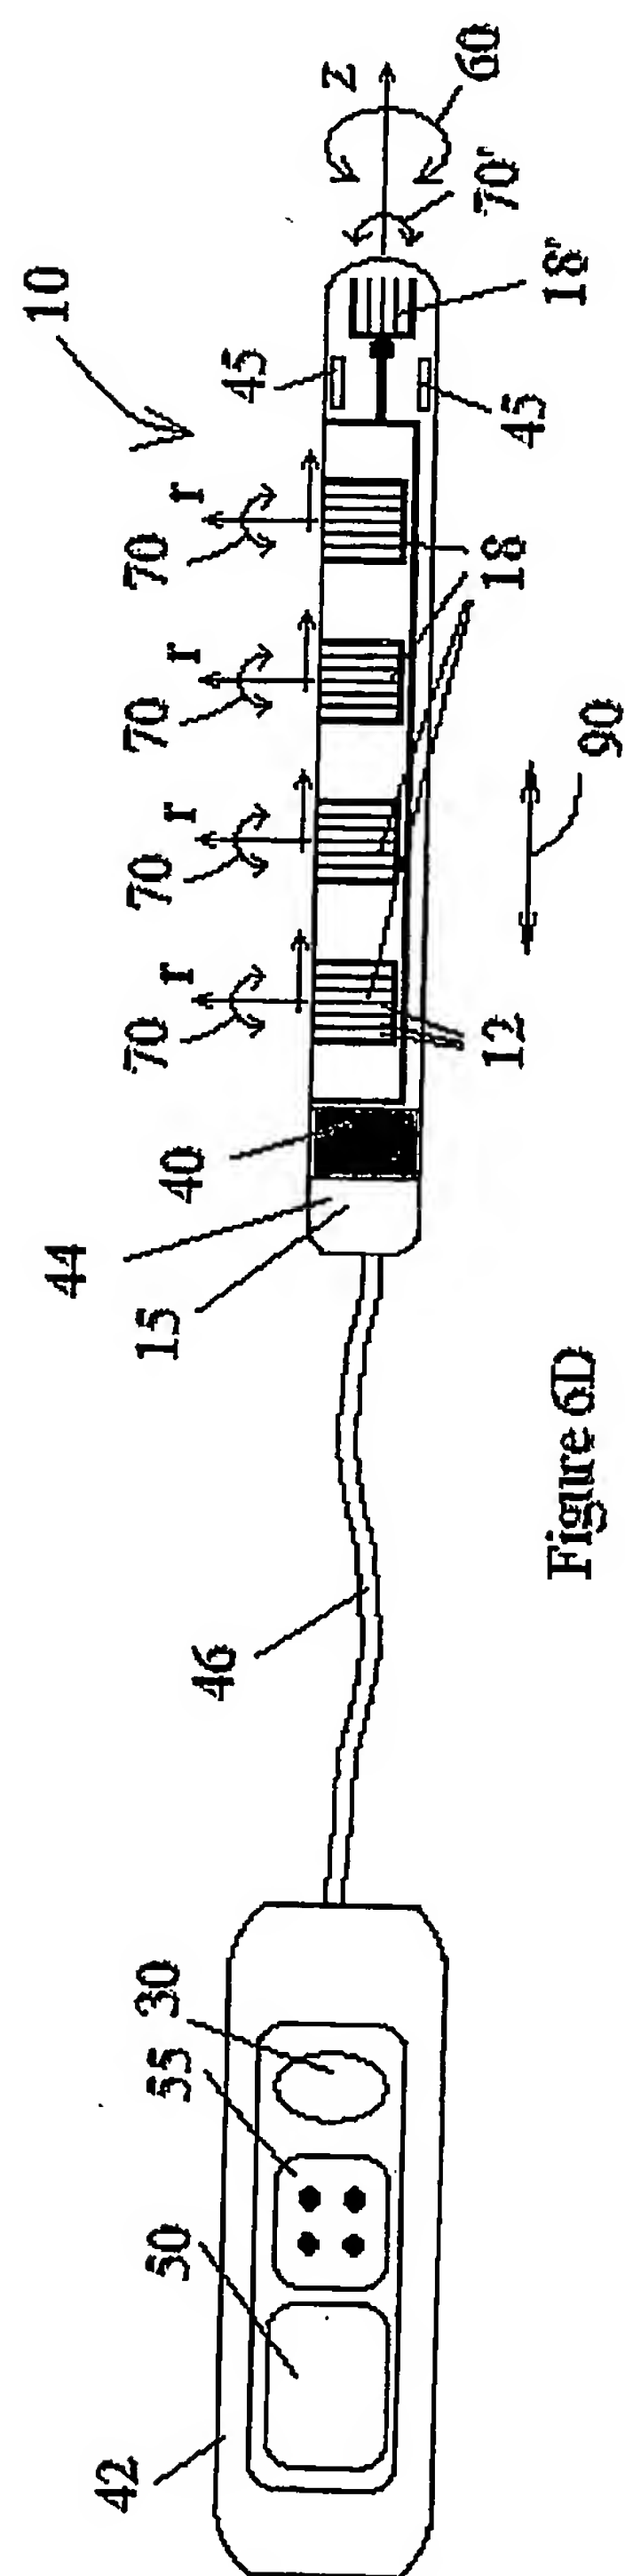



Figure 6B



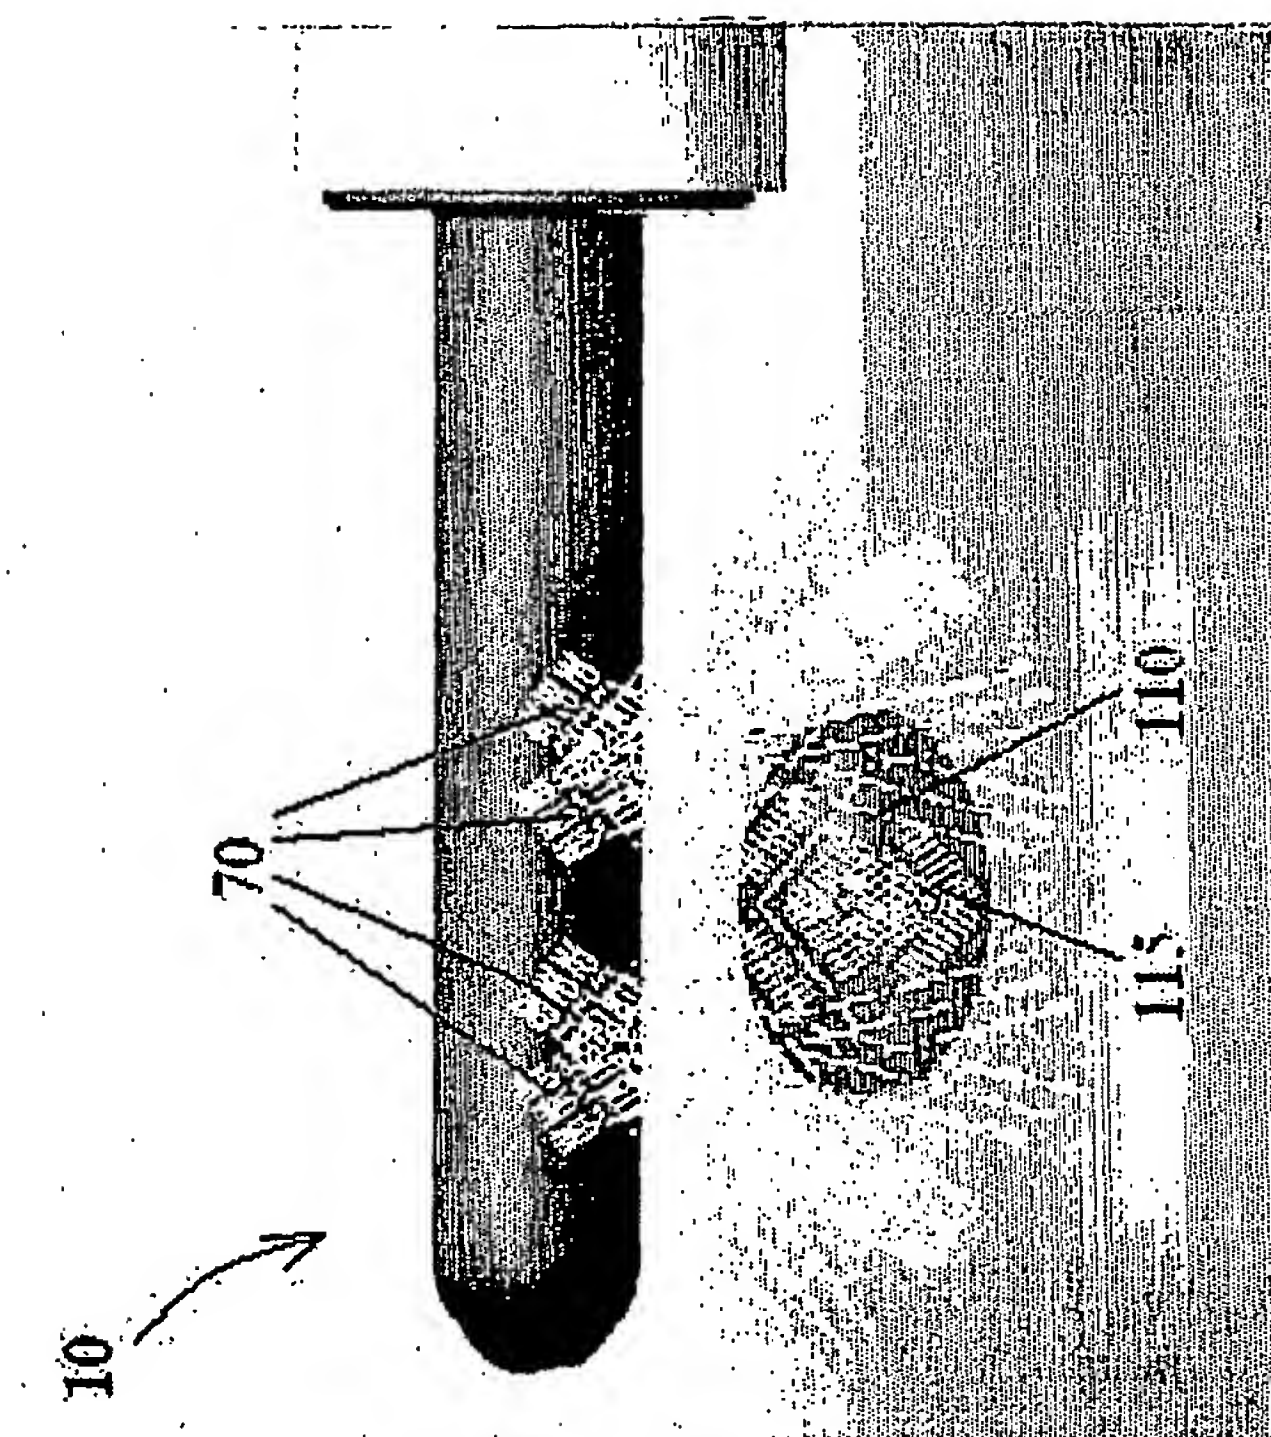


Figure 6F

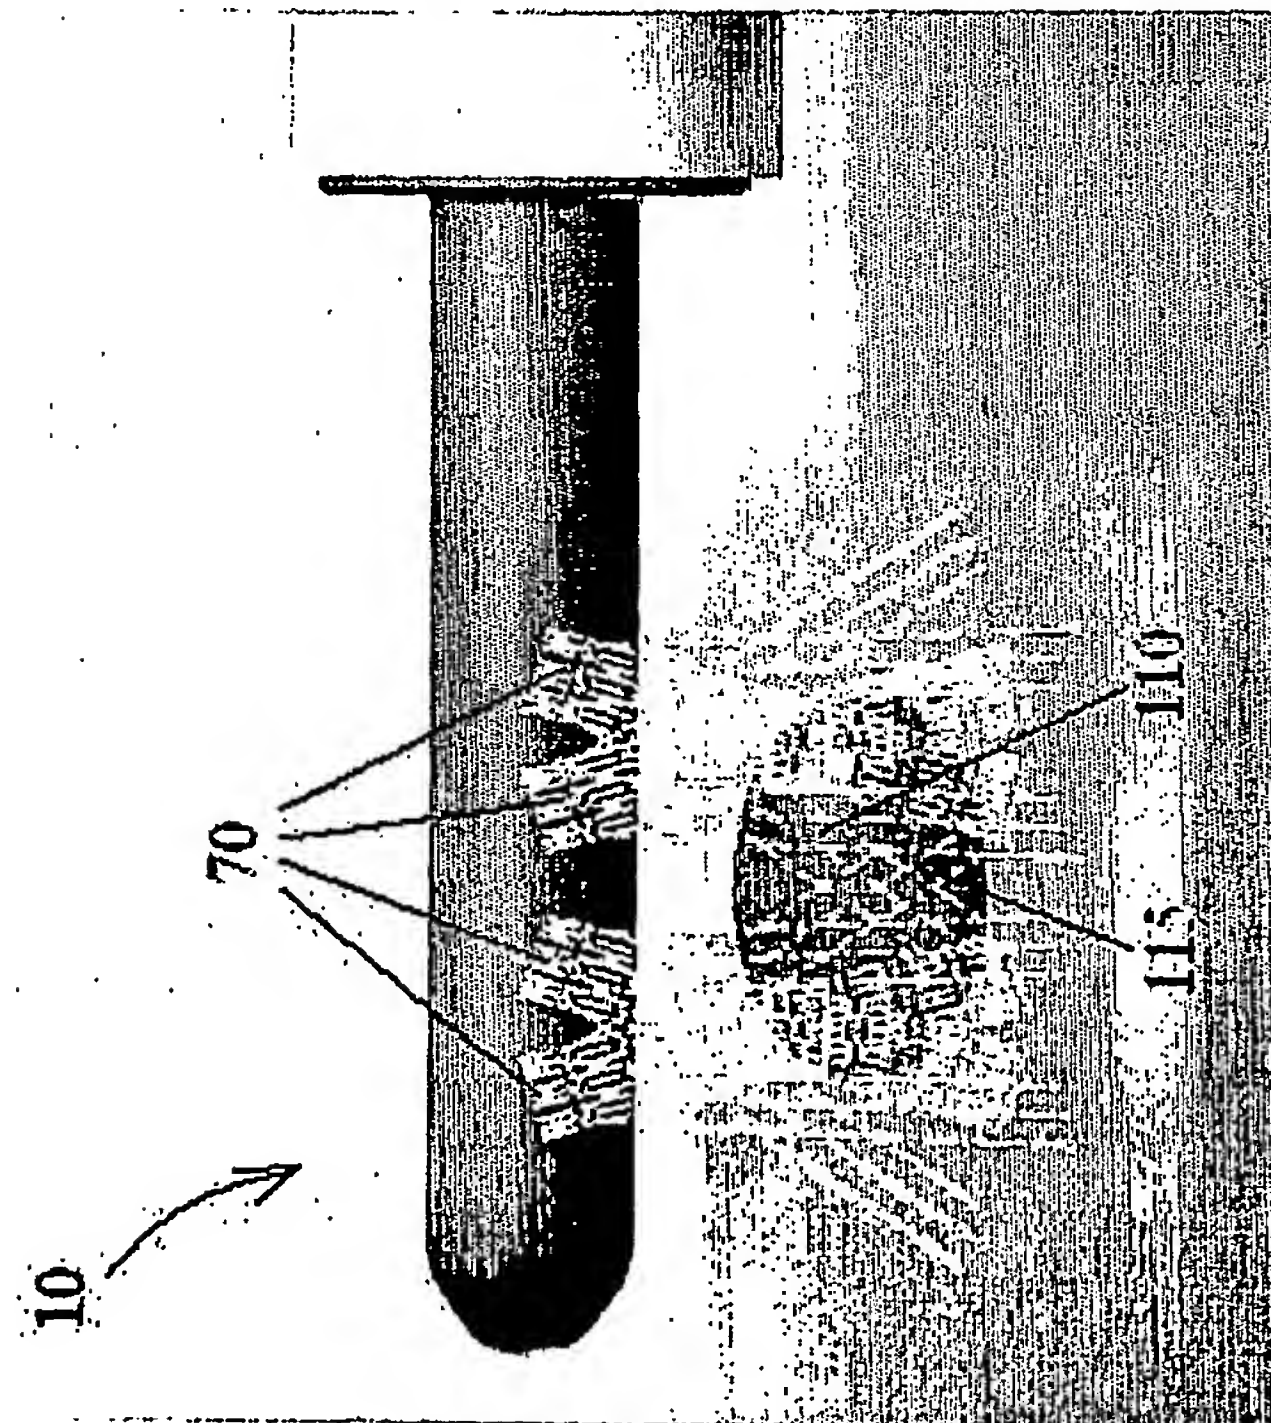


Figure 6E

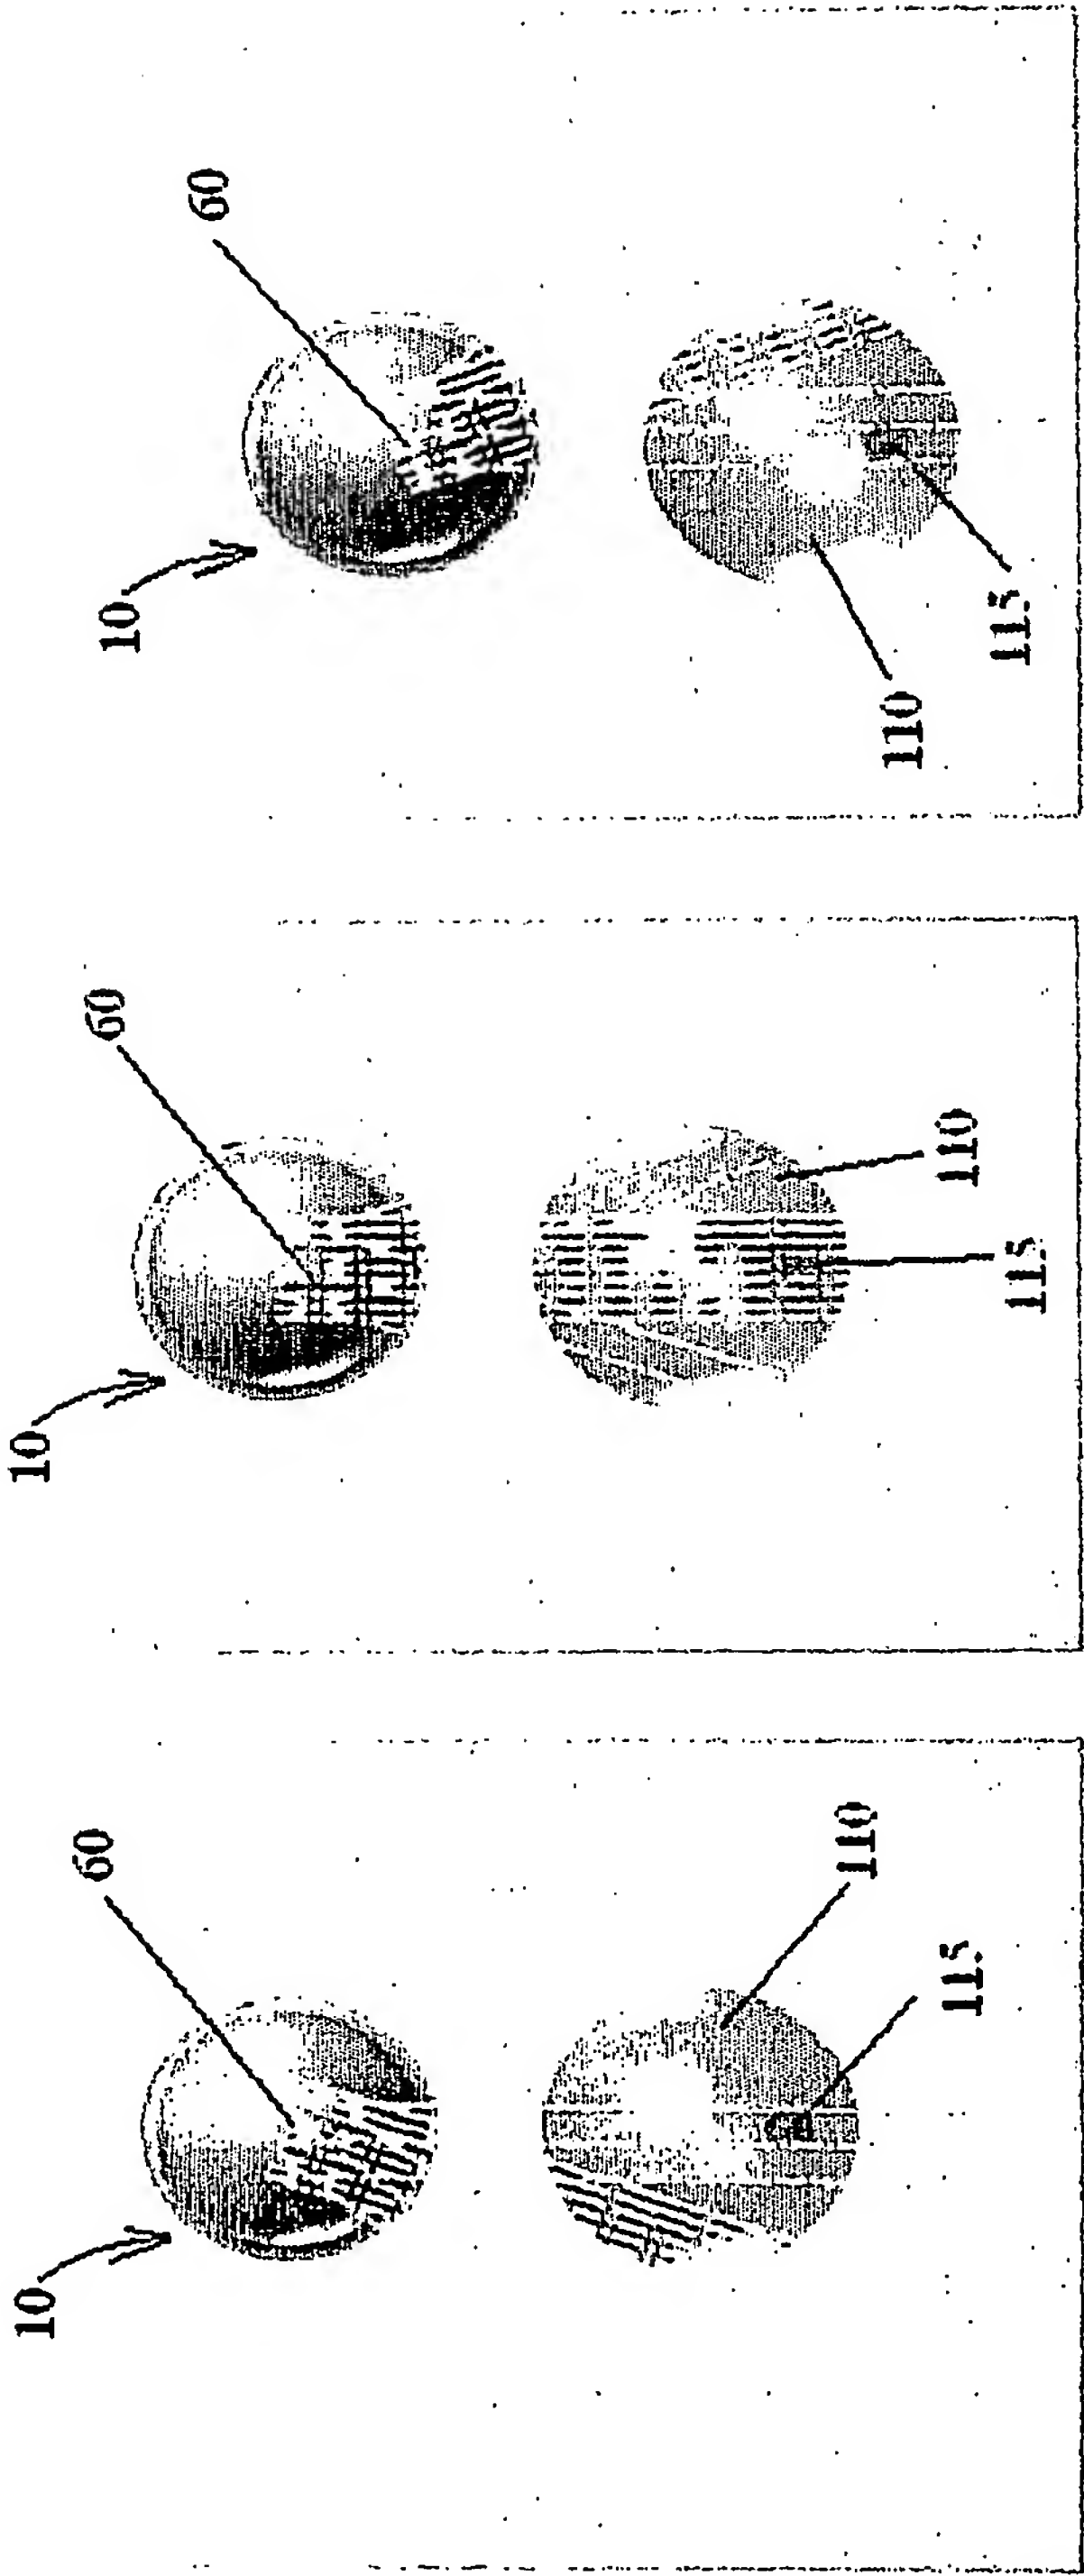


Figure 6I

Figure 6H

Figure 6G

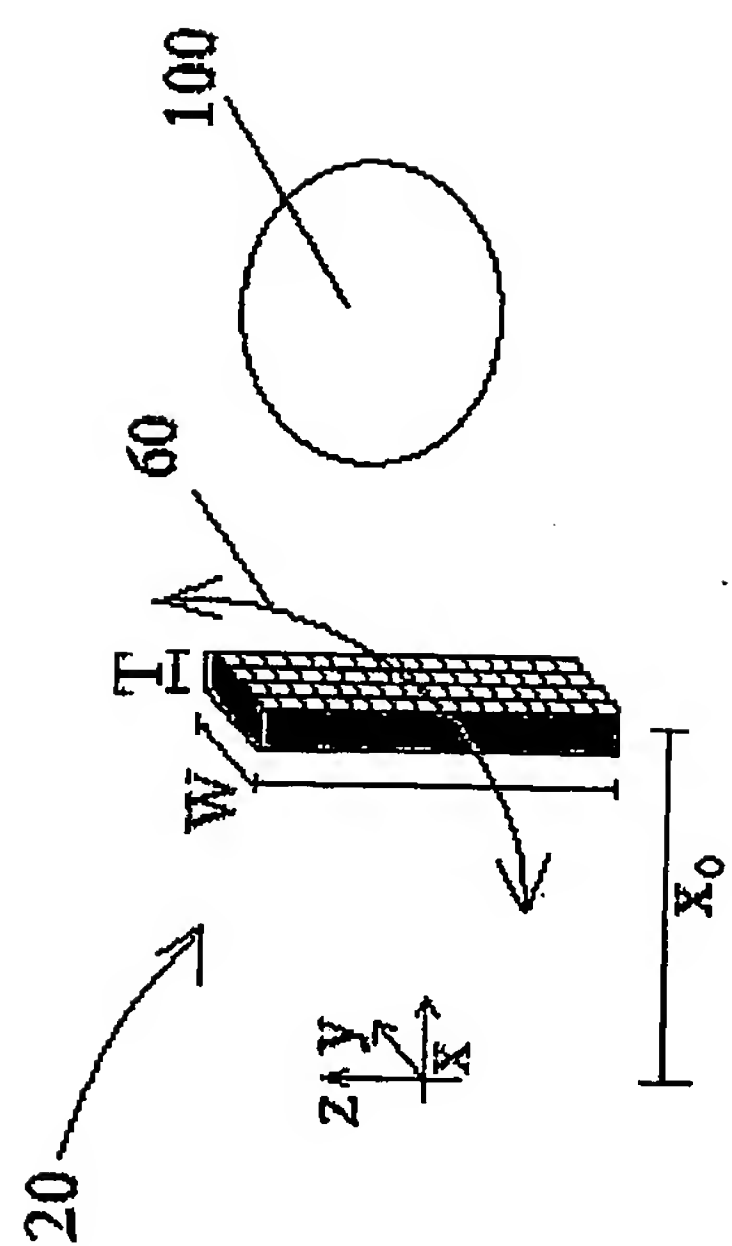


Figure 7

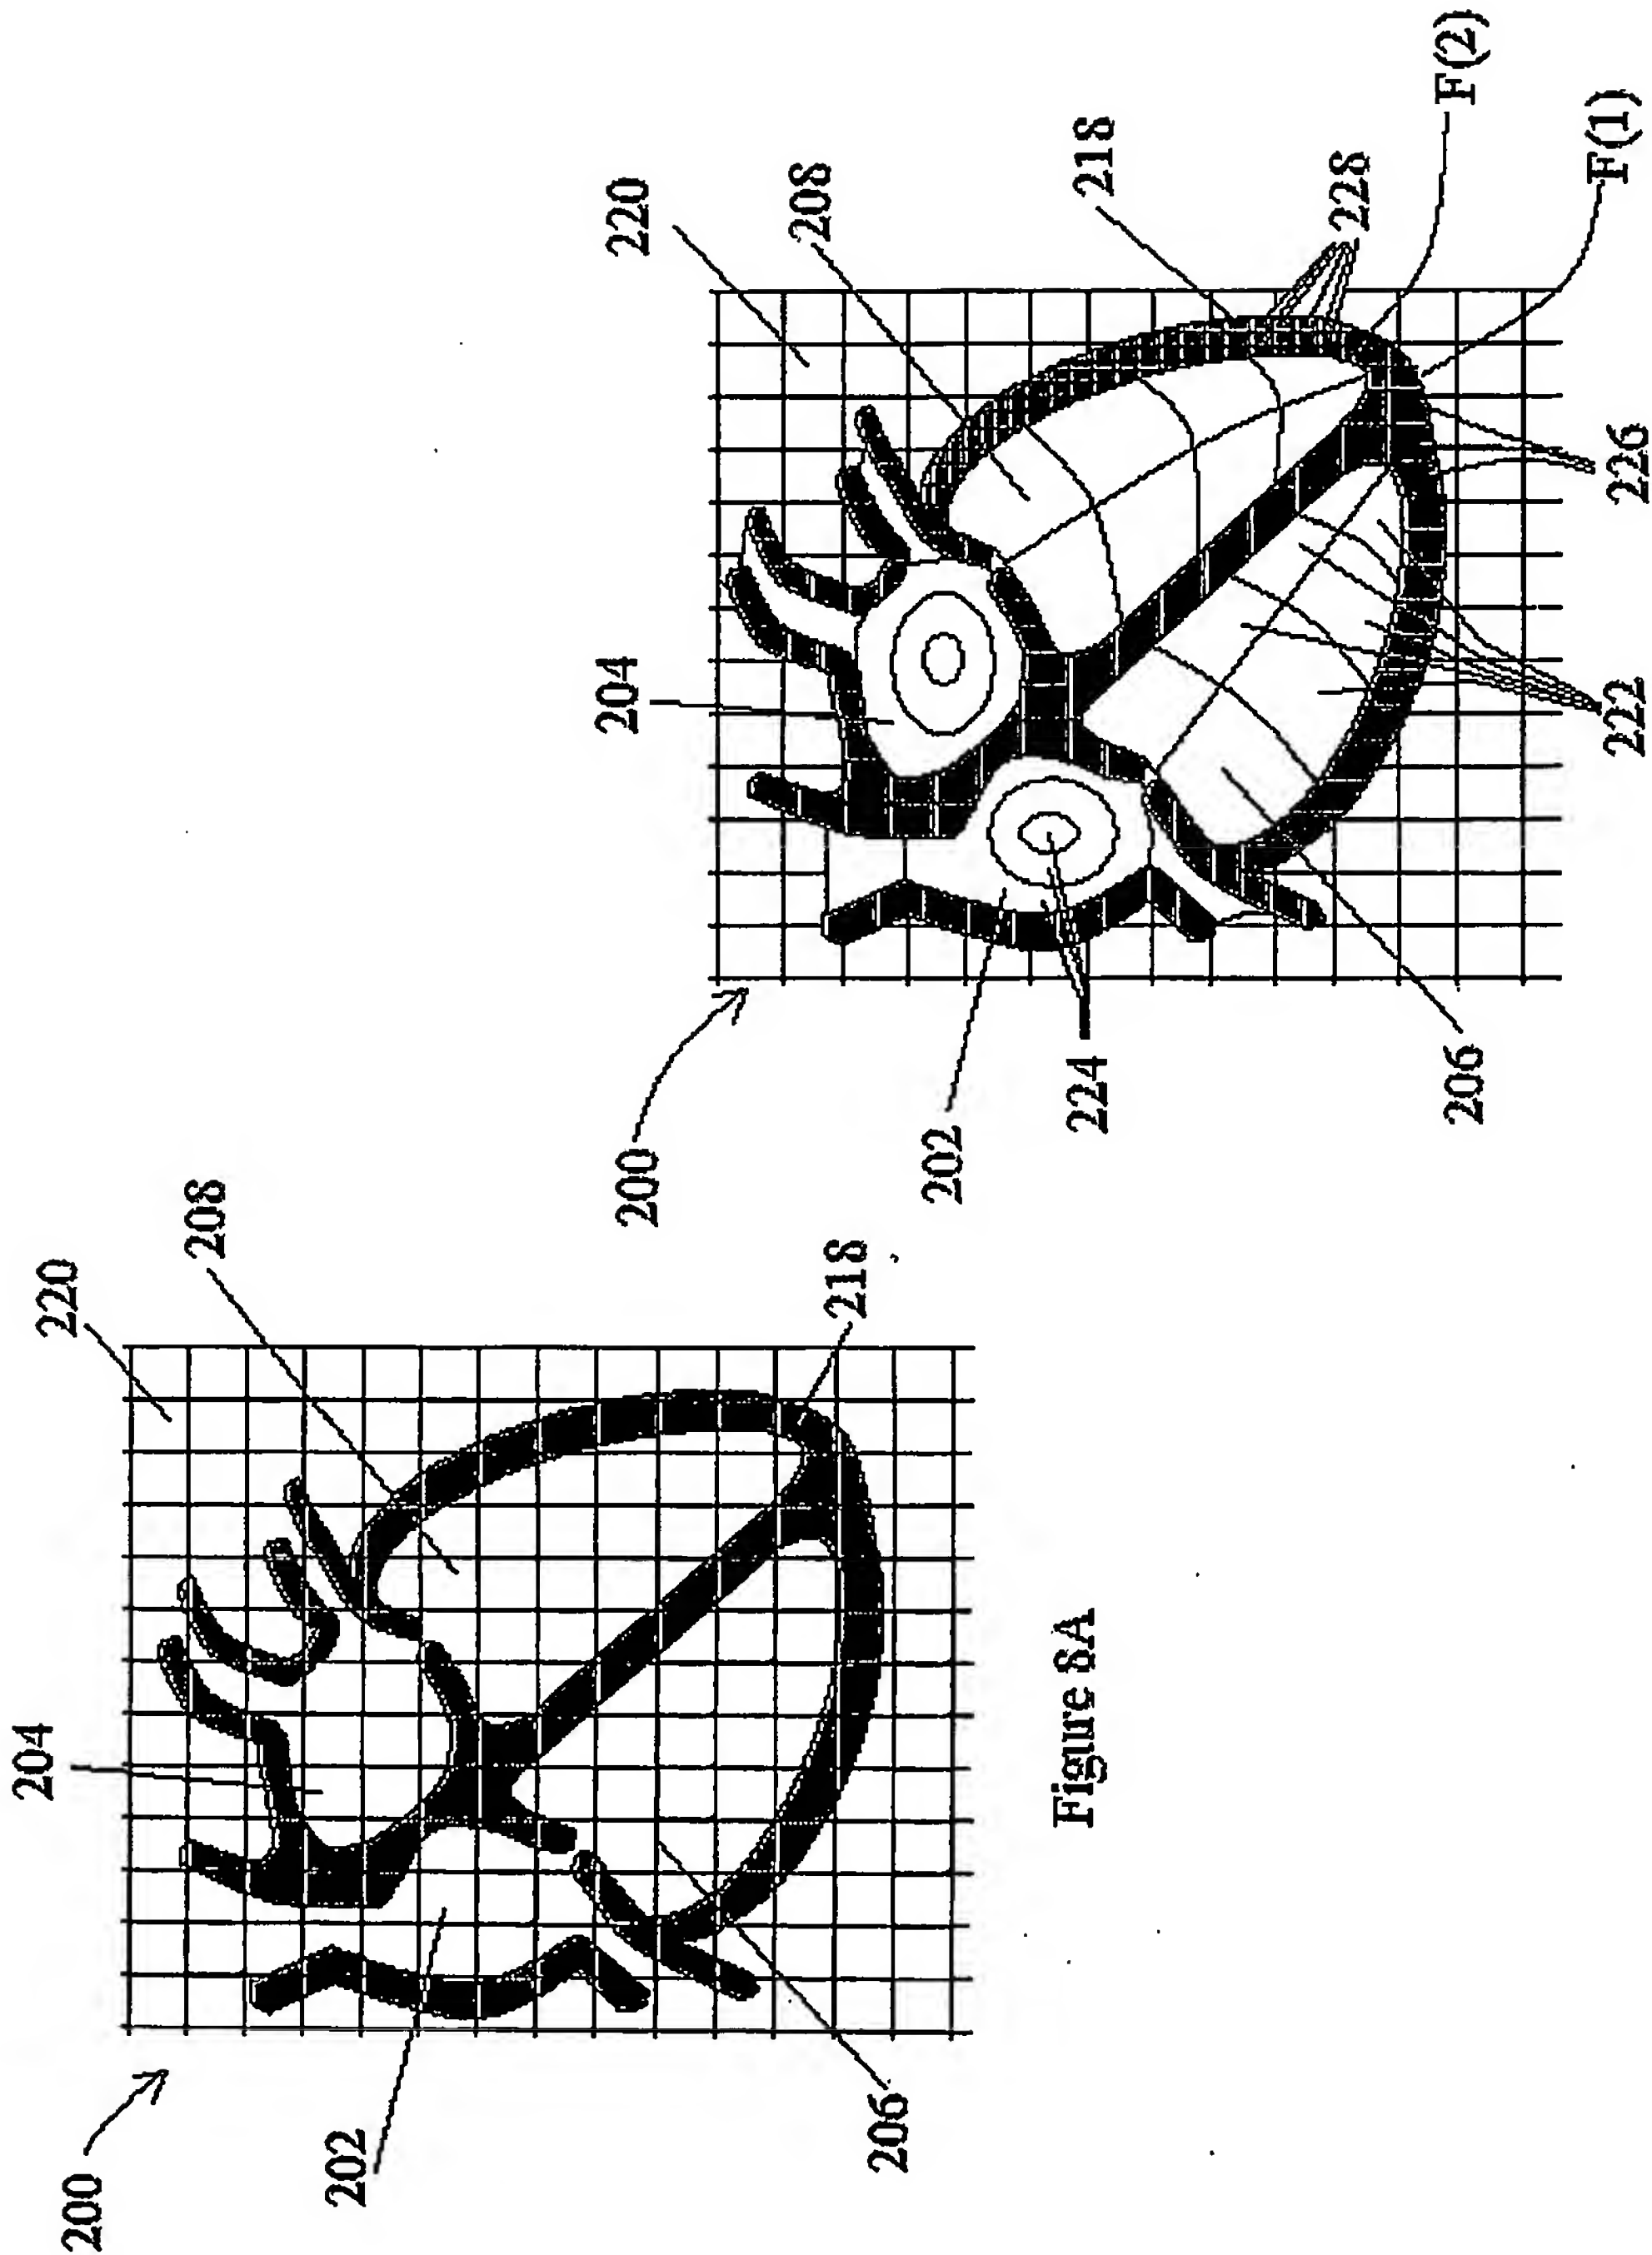


Figure 8B


Figure 8A

Anatomical Landmarks

WO 2007/054935

13/25

PCT/IL2006/001291

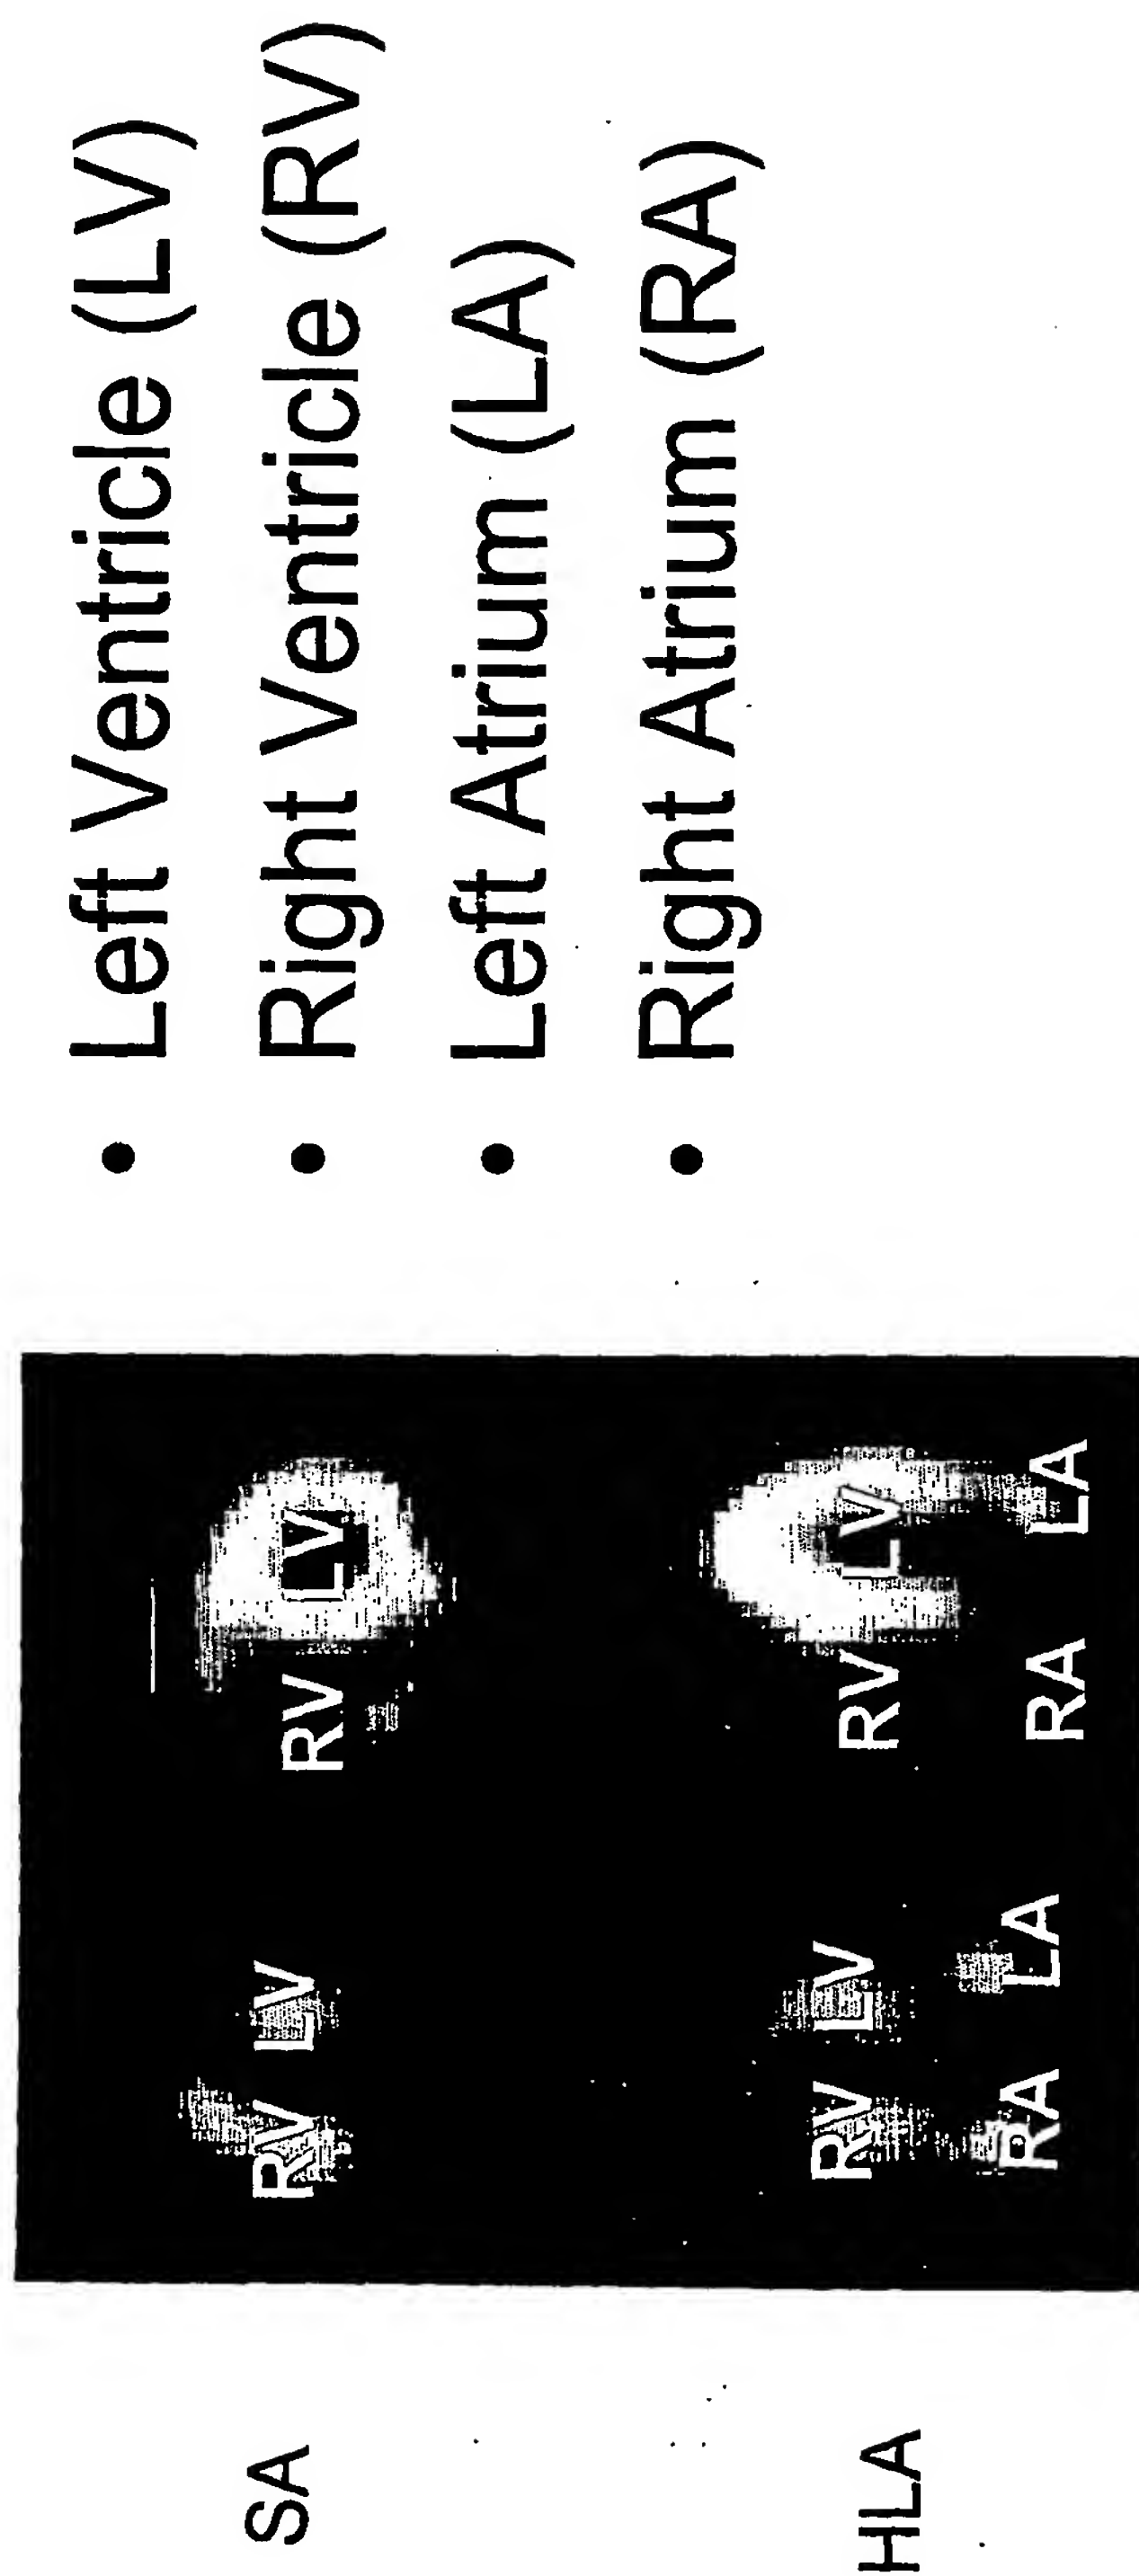

- Left Ventricle (LV)
- Right Ventricle (RV)
- Left Atrium (LA)
- Right Atrium (RA)

Blood Pool Myocardium

Figure 9A


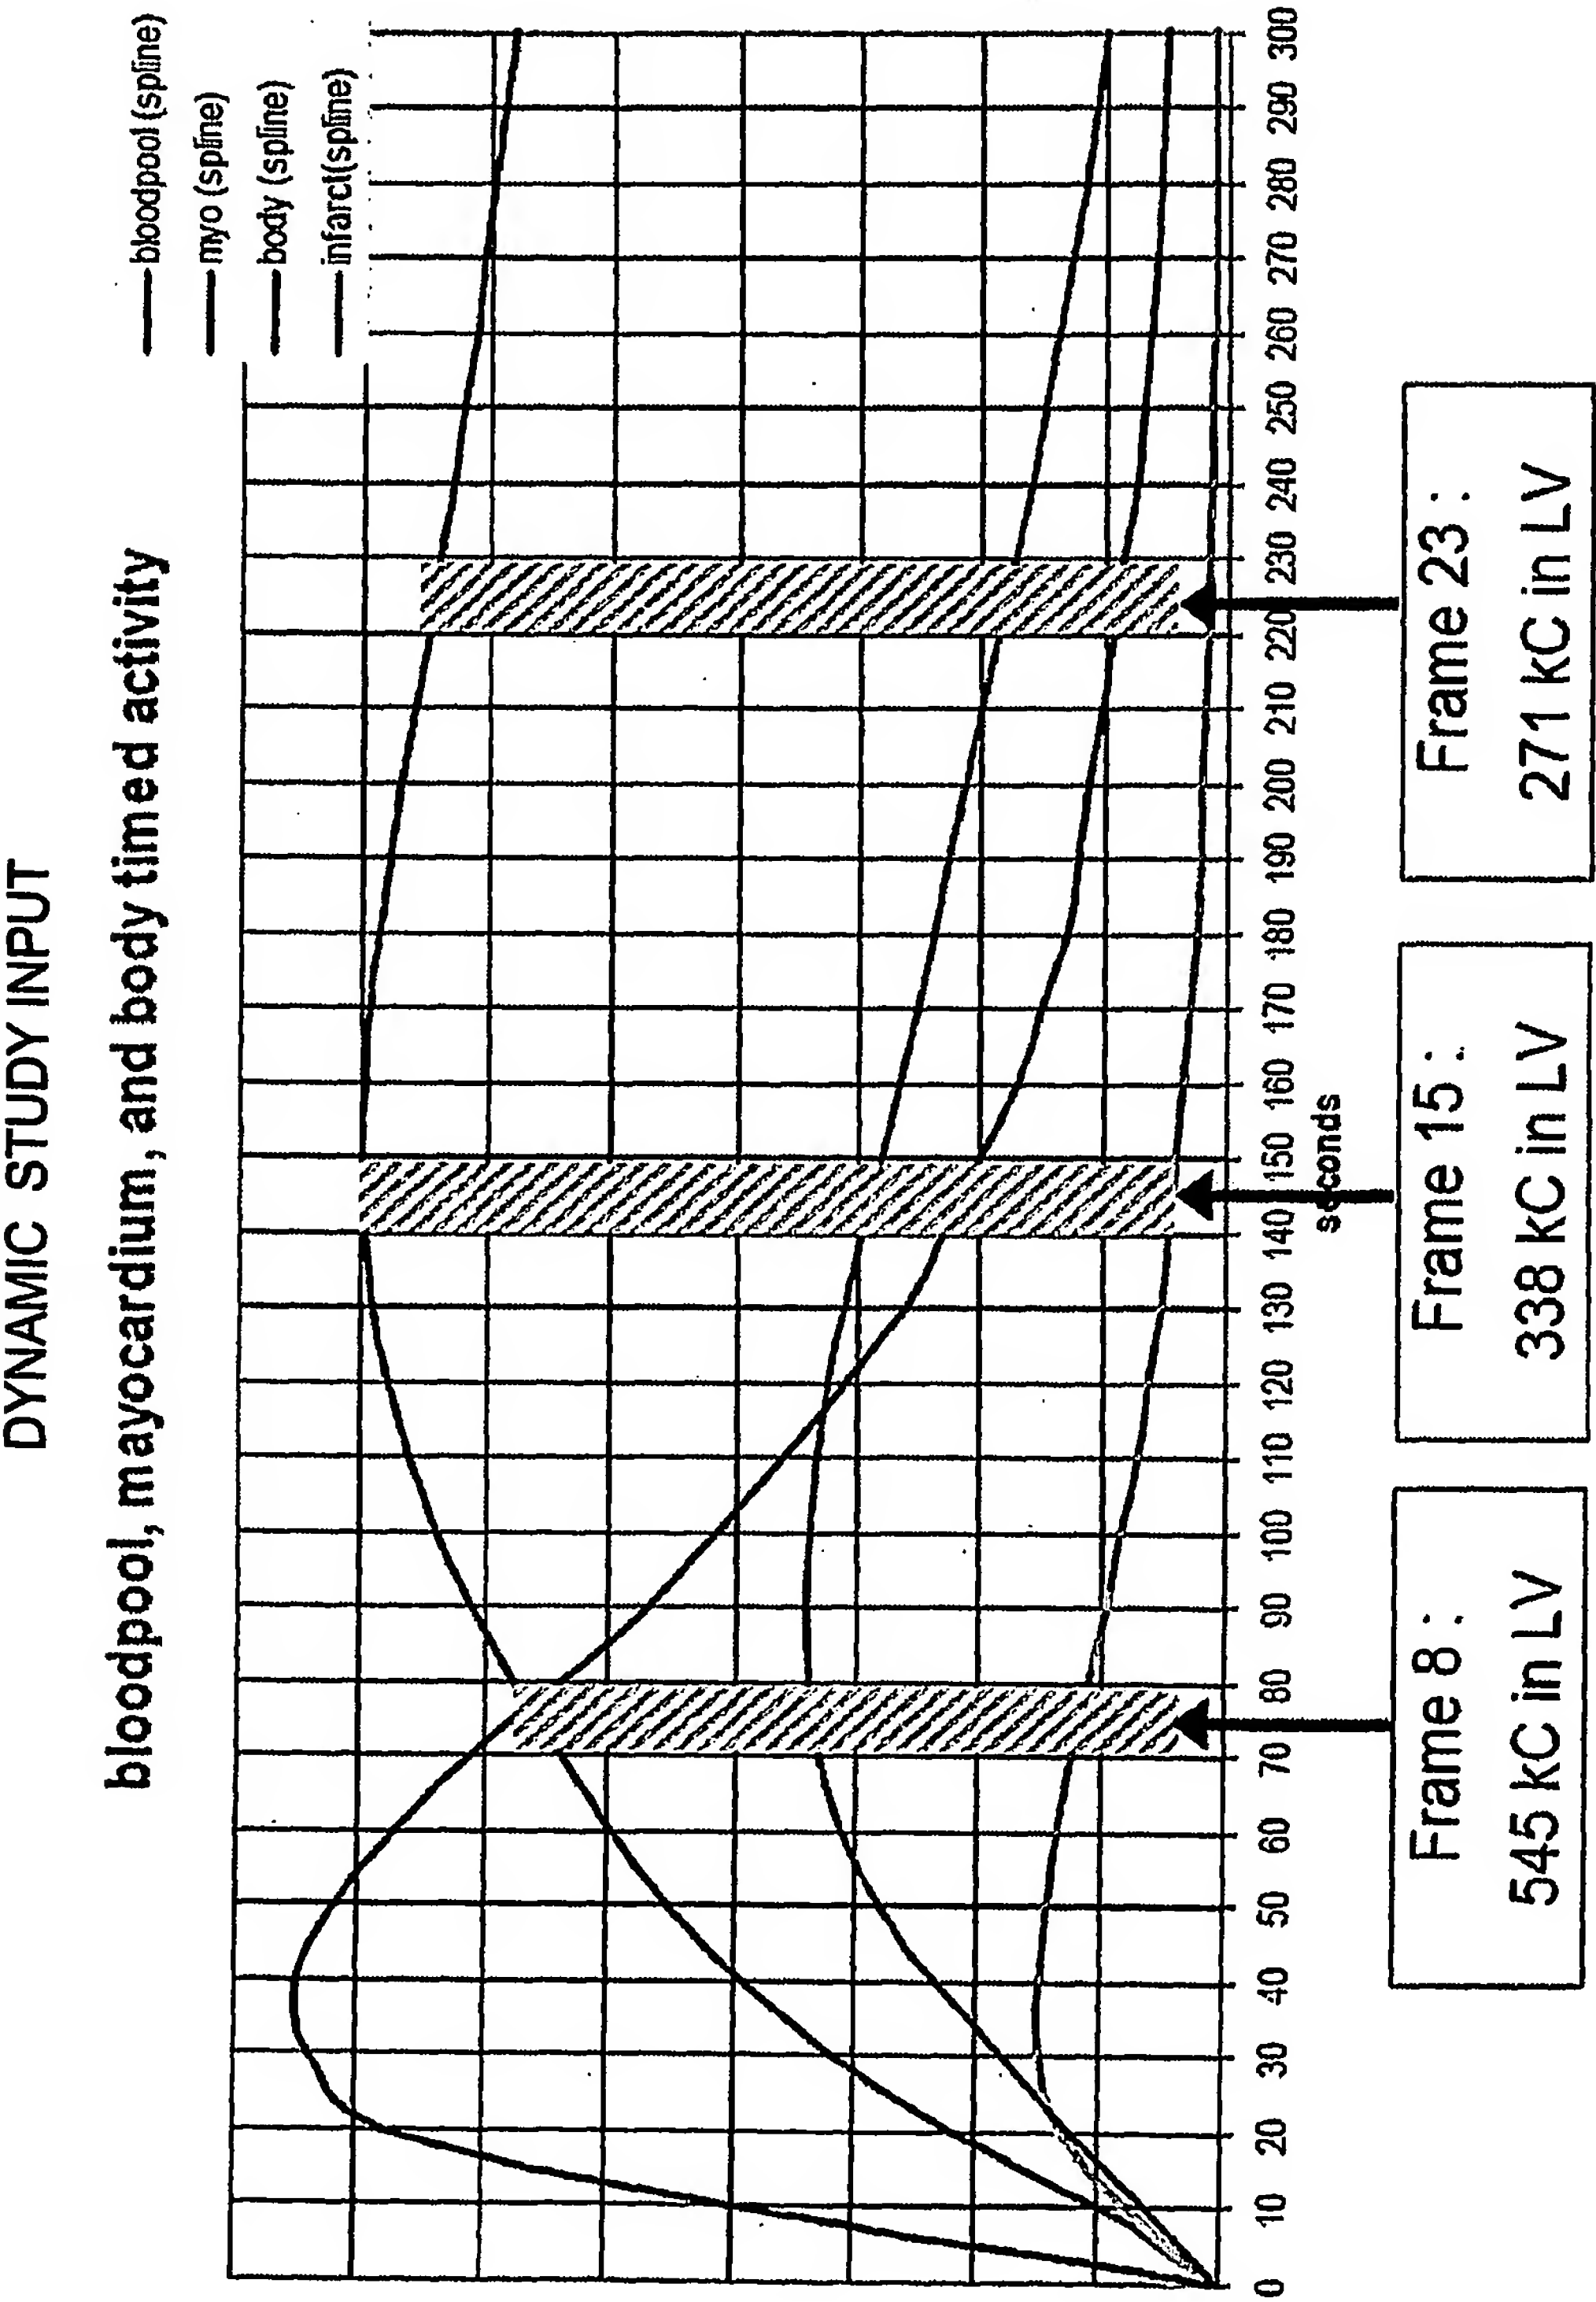


Figure 9B


“Film-stripe” representation of a dynamic SPECT study

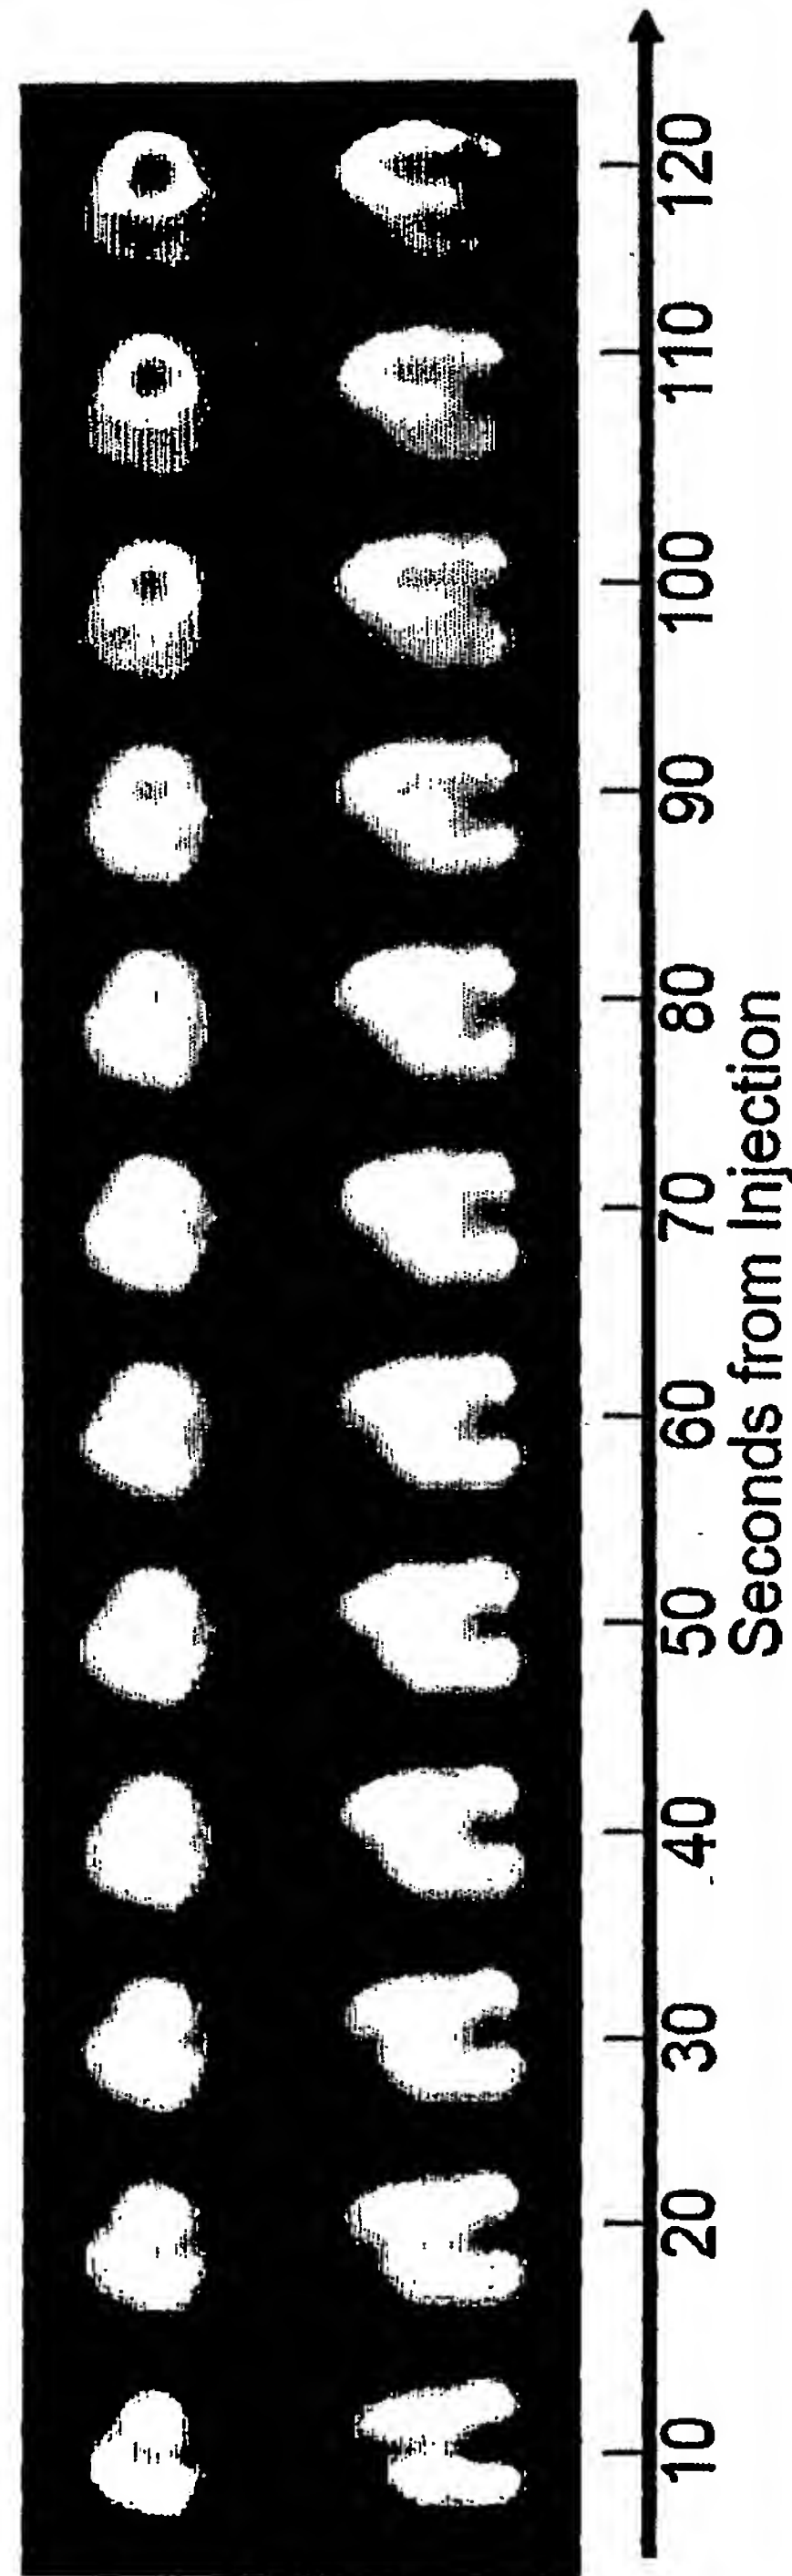

- First 2 minutes after Tc99m-Teboroxime* injection, 10s/frame
- Mid-ventricular slices (upper row : SA lower row: HLA)
- Note as the intense blood pool activity at the center of the heart chambers gradually clears, while the myocardial uptake gradually intensifies.

Figure 9C

“Film-stripe” representation of a dynamic SPECT study

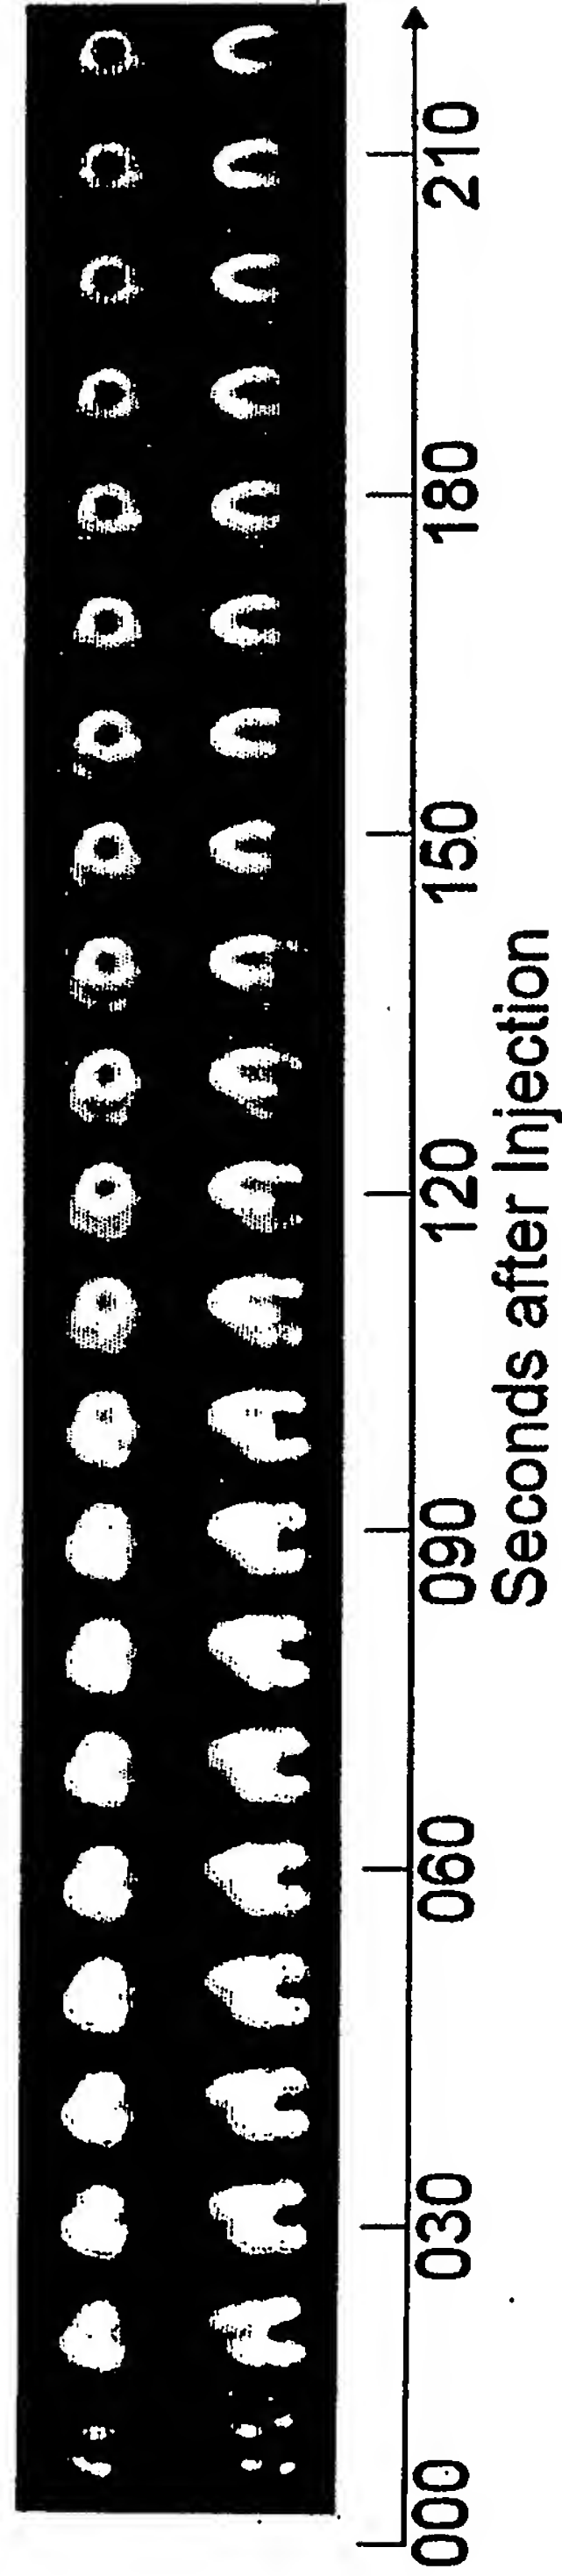

- First 4 minutes after Tc99m-Teboroxime* injection, 10s/frame
- Mid-ventricular slices (upper row : SA lower row: HLA)
- Note as the intense blood pool activity at the center of the heart chambers gradually clears, while the myocardial uptake gradually intensifies

Figure 9D

“Movie” representation of a dynamic SPECT study (SA)

- First 4 minutes after Tc99m-Teboroxime* injection, 10s/frame
- Mid-ventricular SA slices.
- Note as the intense blood pool activity gradually clears in LV and RV cavities
- Myocardial uptake gradually intensifies, (the thin walled RV is less intense)



Figure 9E

“Movie” representation of a dynamic SPECT study (SA)

- First 4 minutes after Tc99m-Teboroxime* injection, 10s/frame
- Mid-ventricular SA slices.
- Note as the intense blood pool activity gradually clears in LV, RV, LA and RA cavities
- Myocardial uptake gradually intensifies, (the thin walled RV ant atria are less intense)

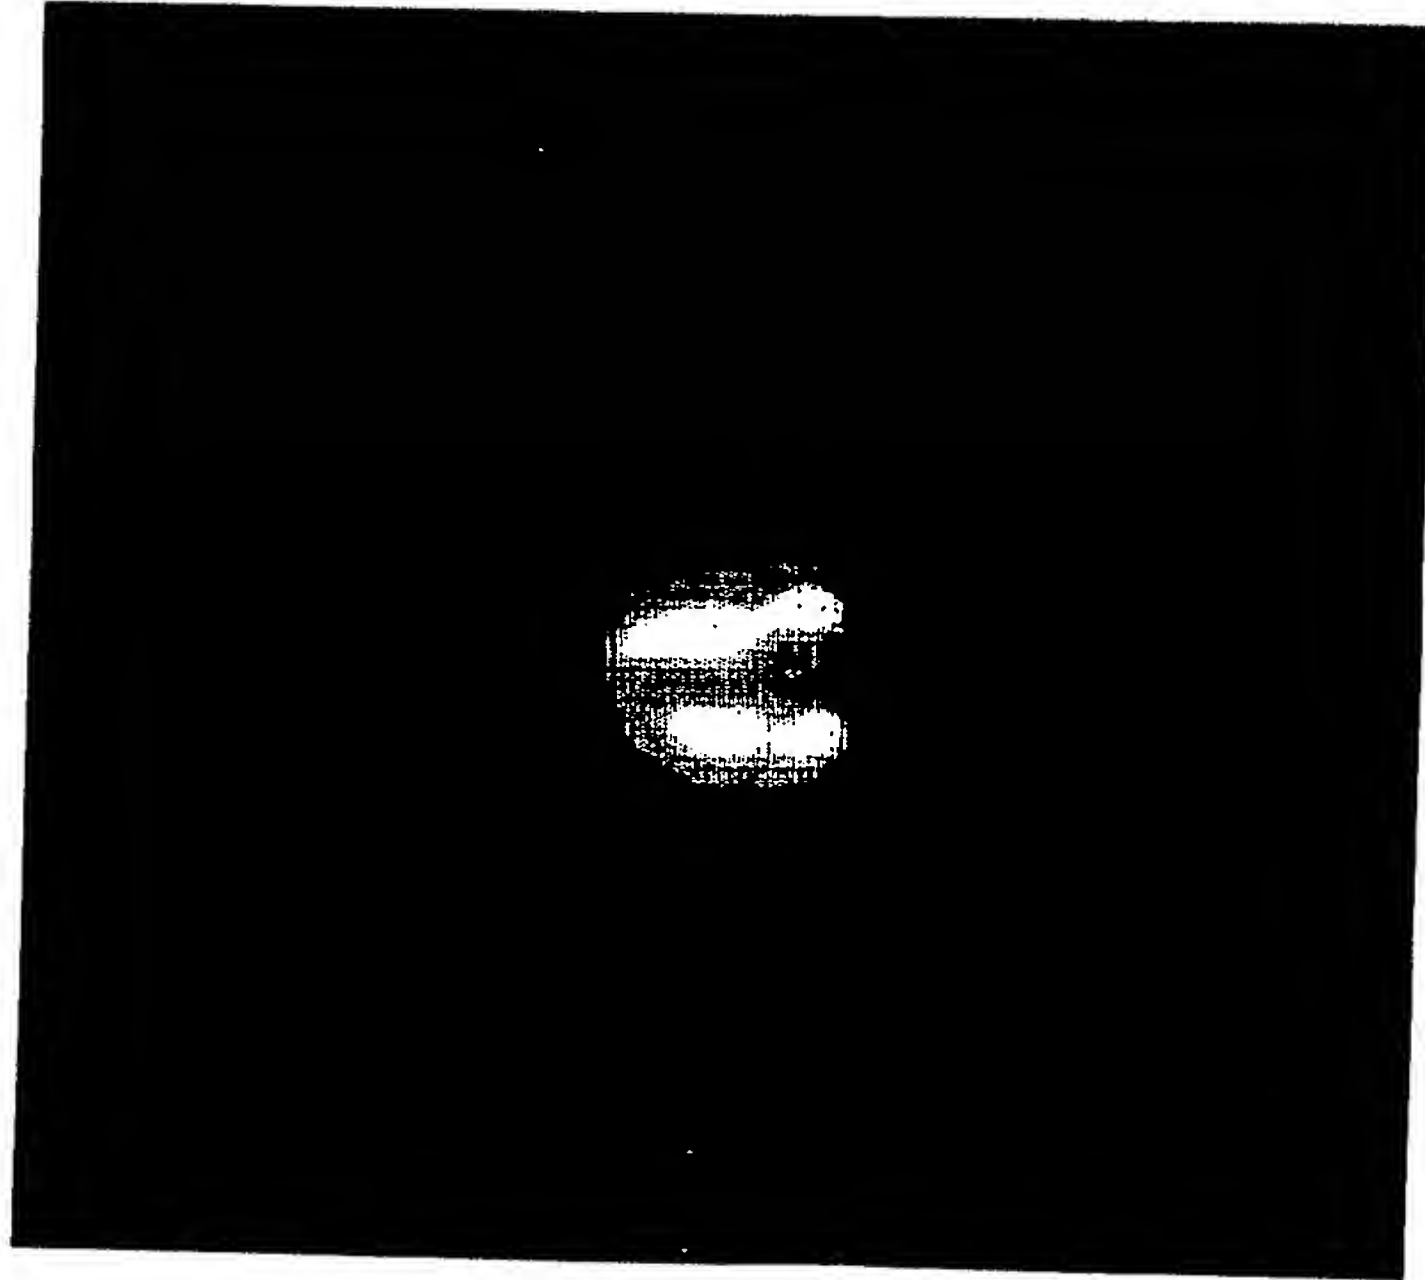


Figure 9F

“Movie” representation of a
dynamic SPECT study (fast)

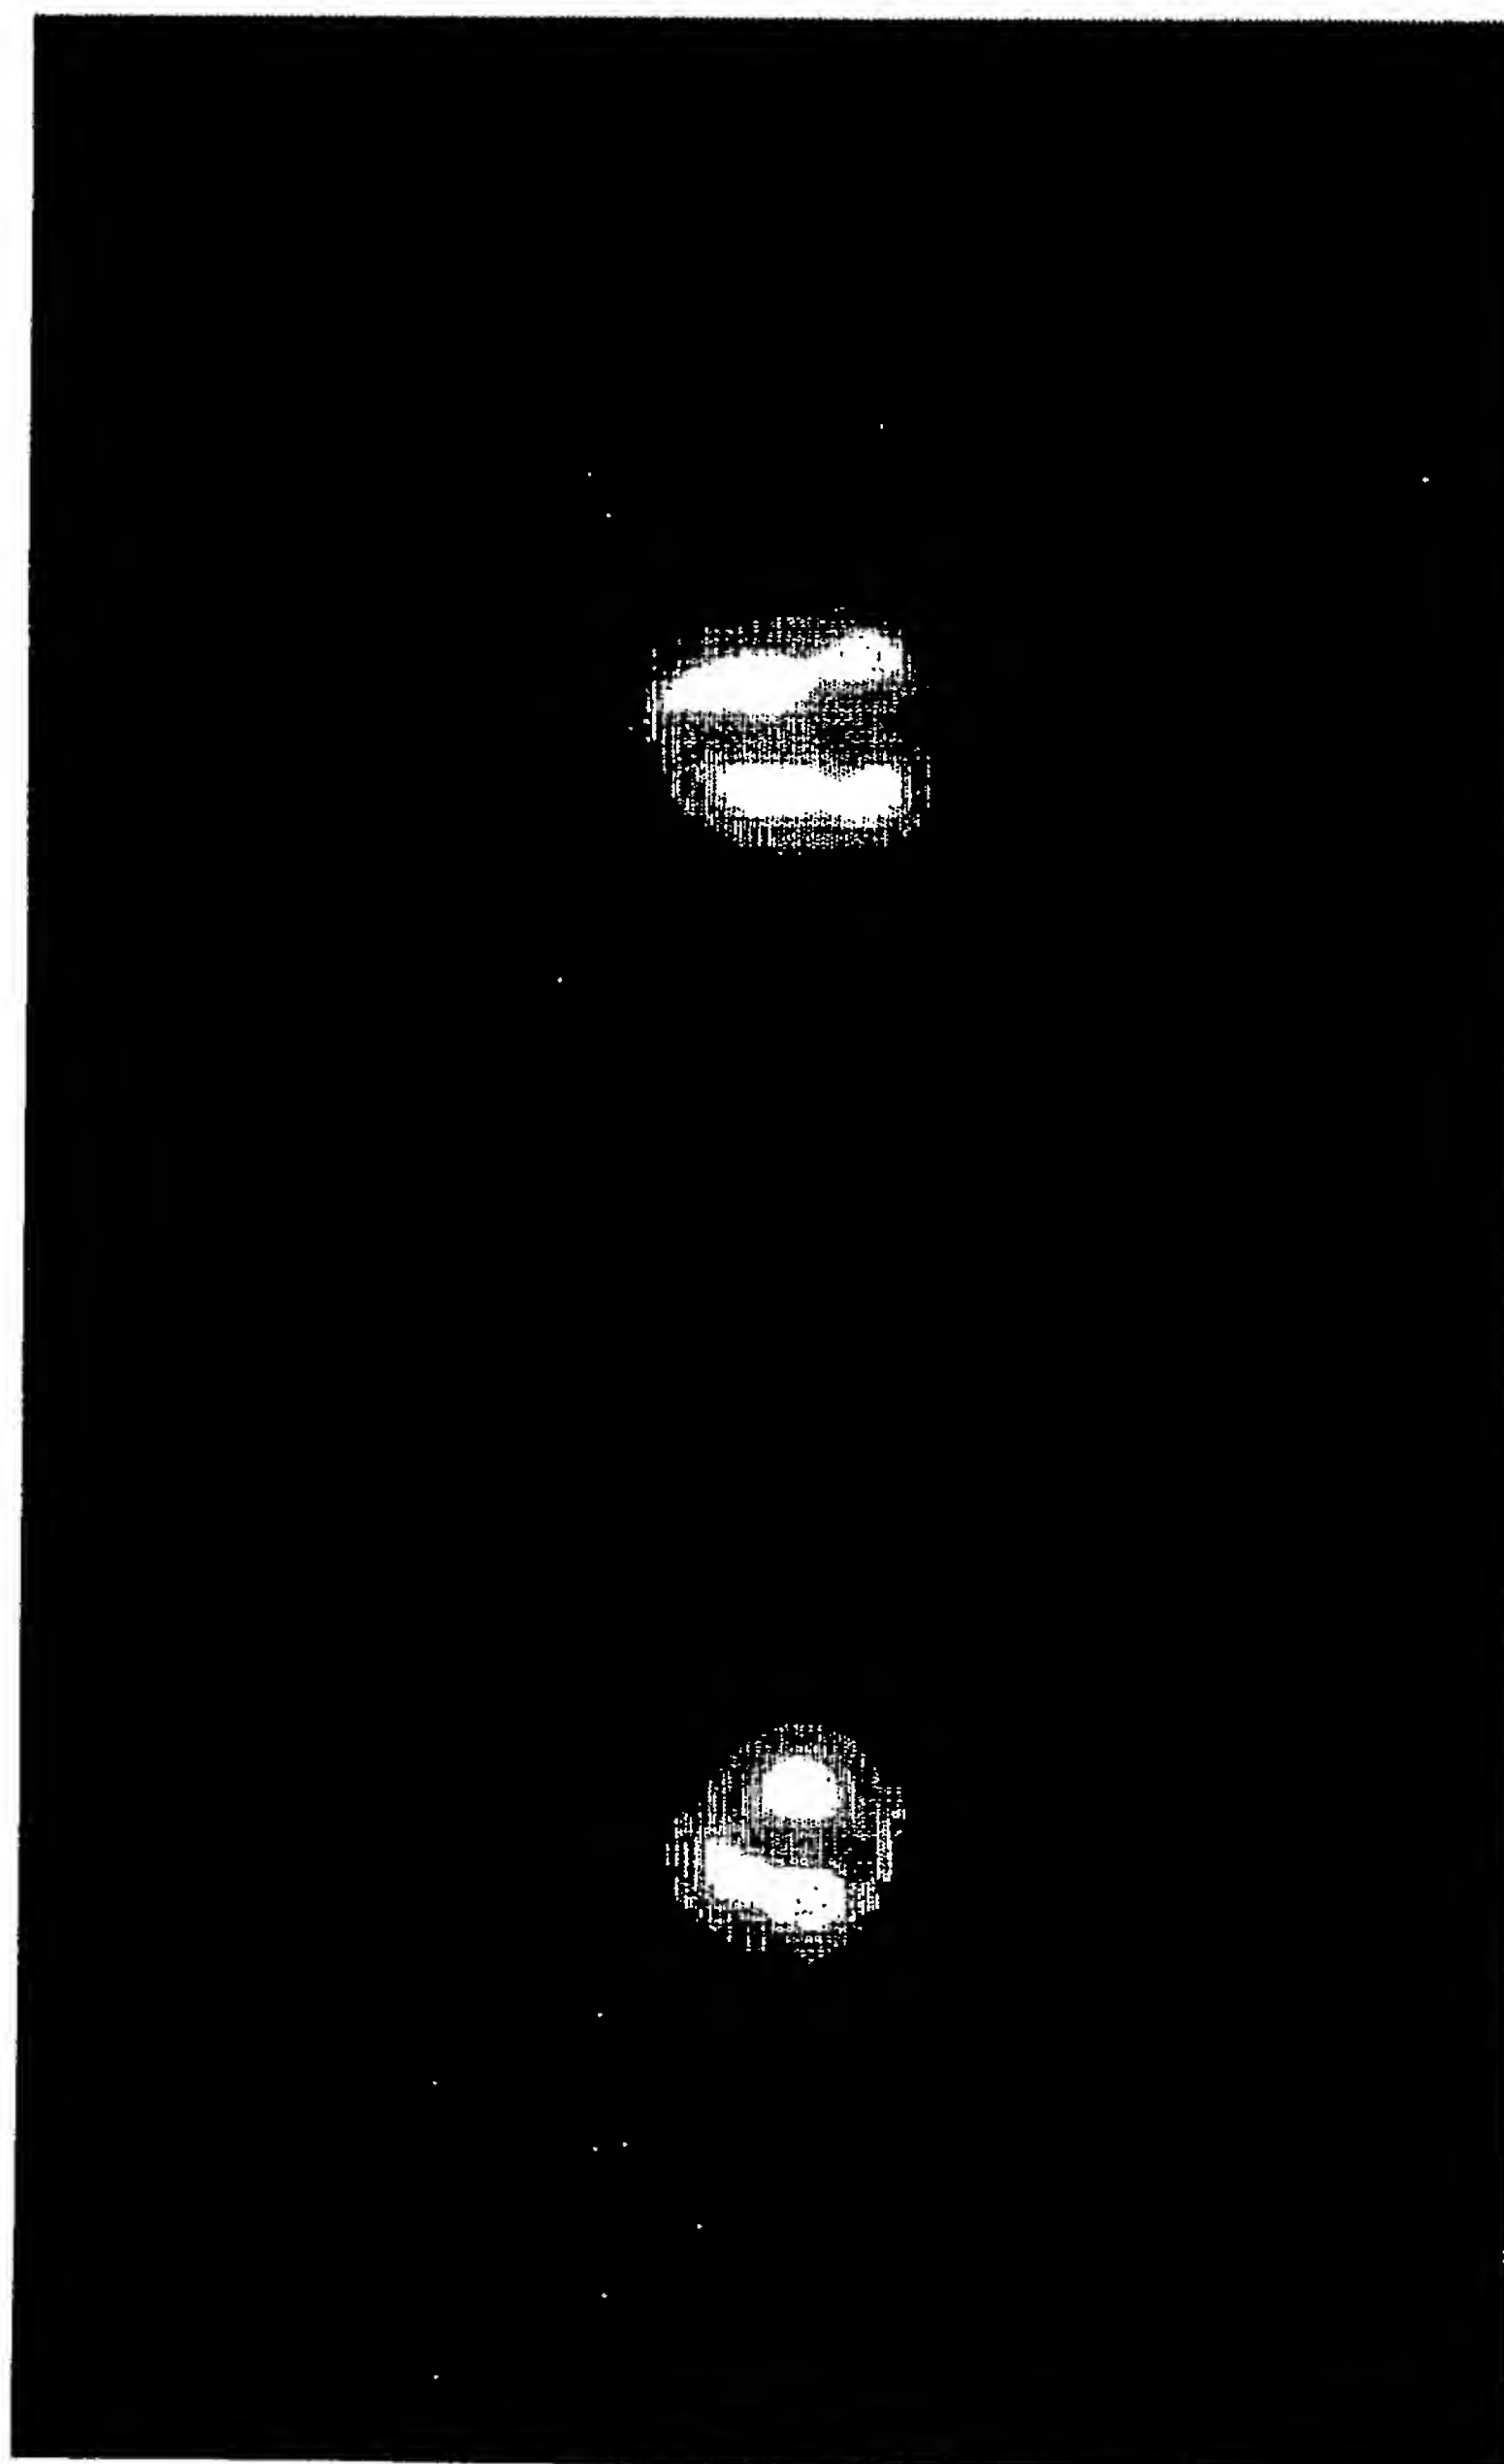


Figure 9G

**“Movie” representation of a
dynamic SPECT study (slow)**

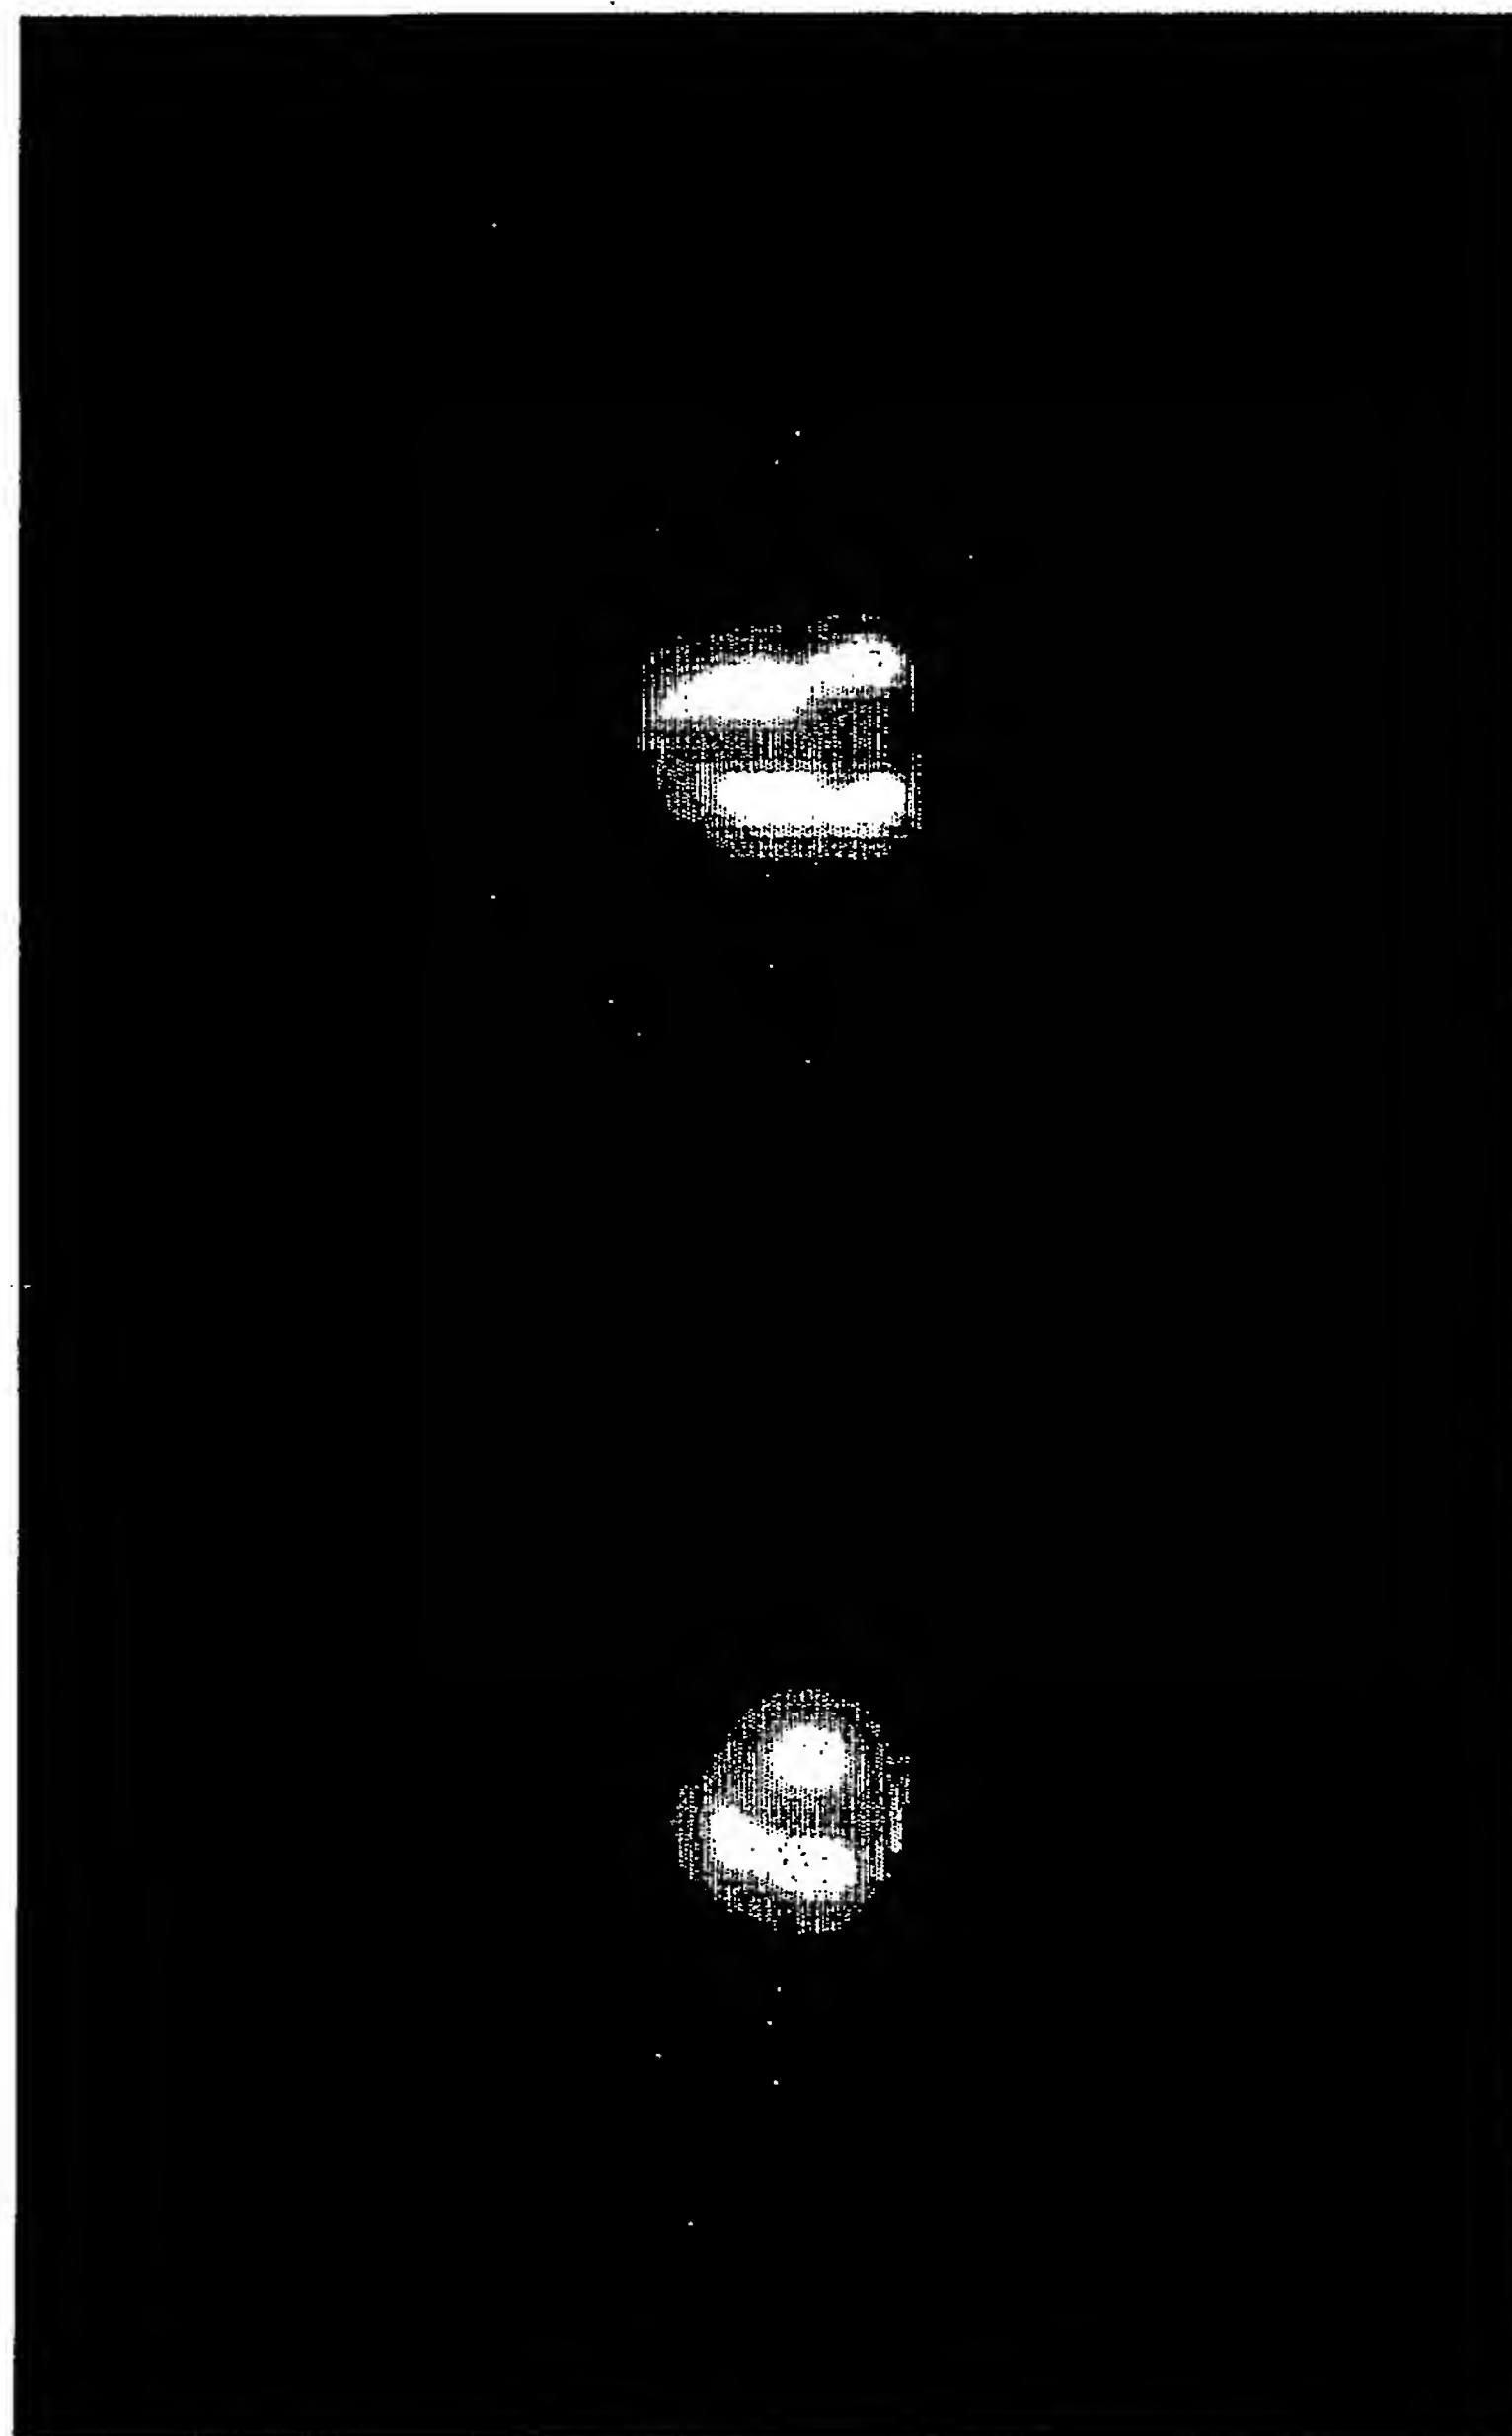


Figure 9H

Volume Segmentation for separate tissue flow dynamics measurement

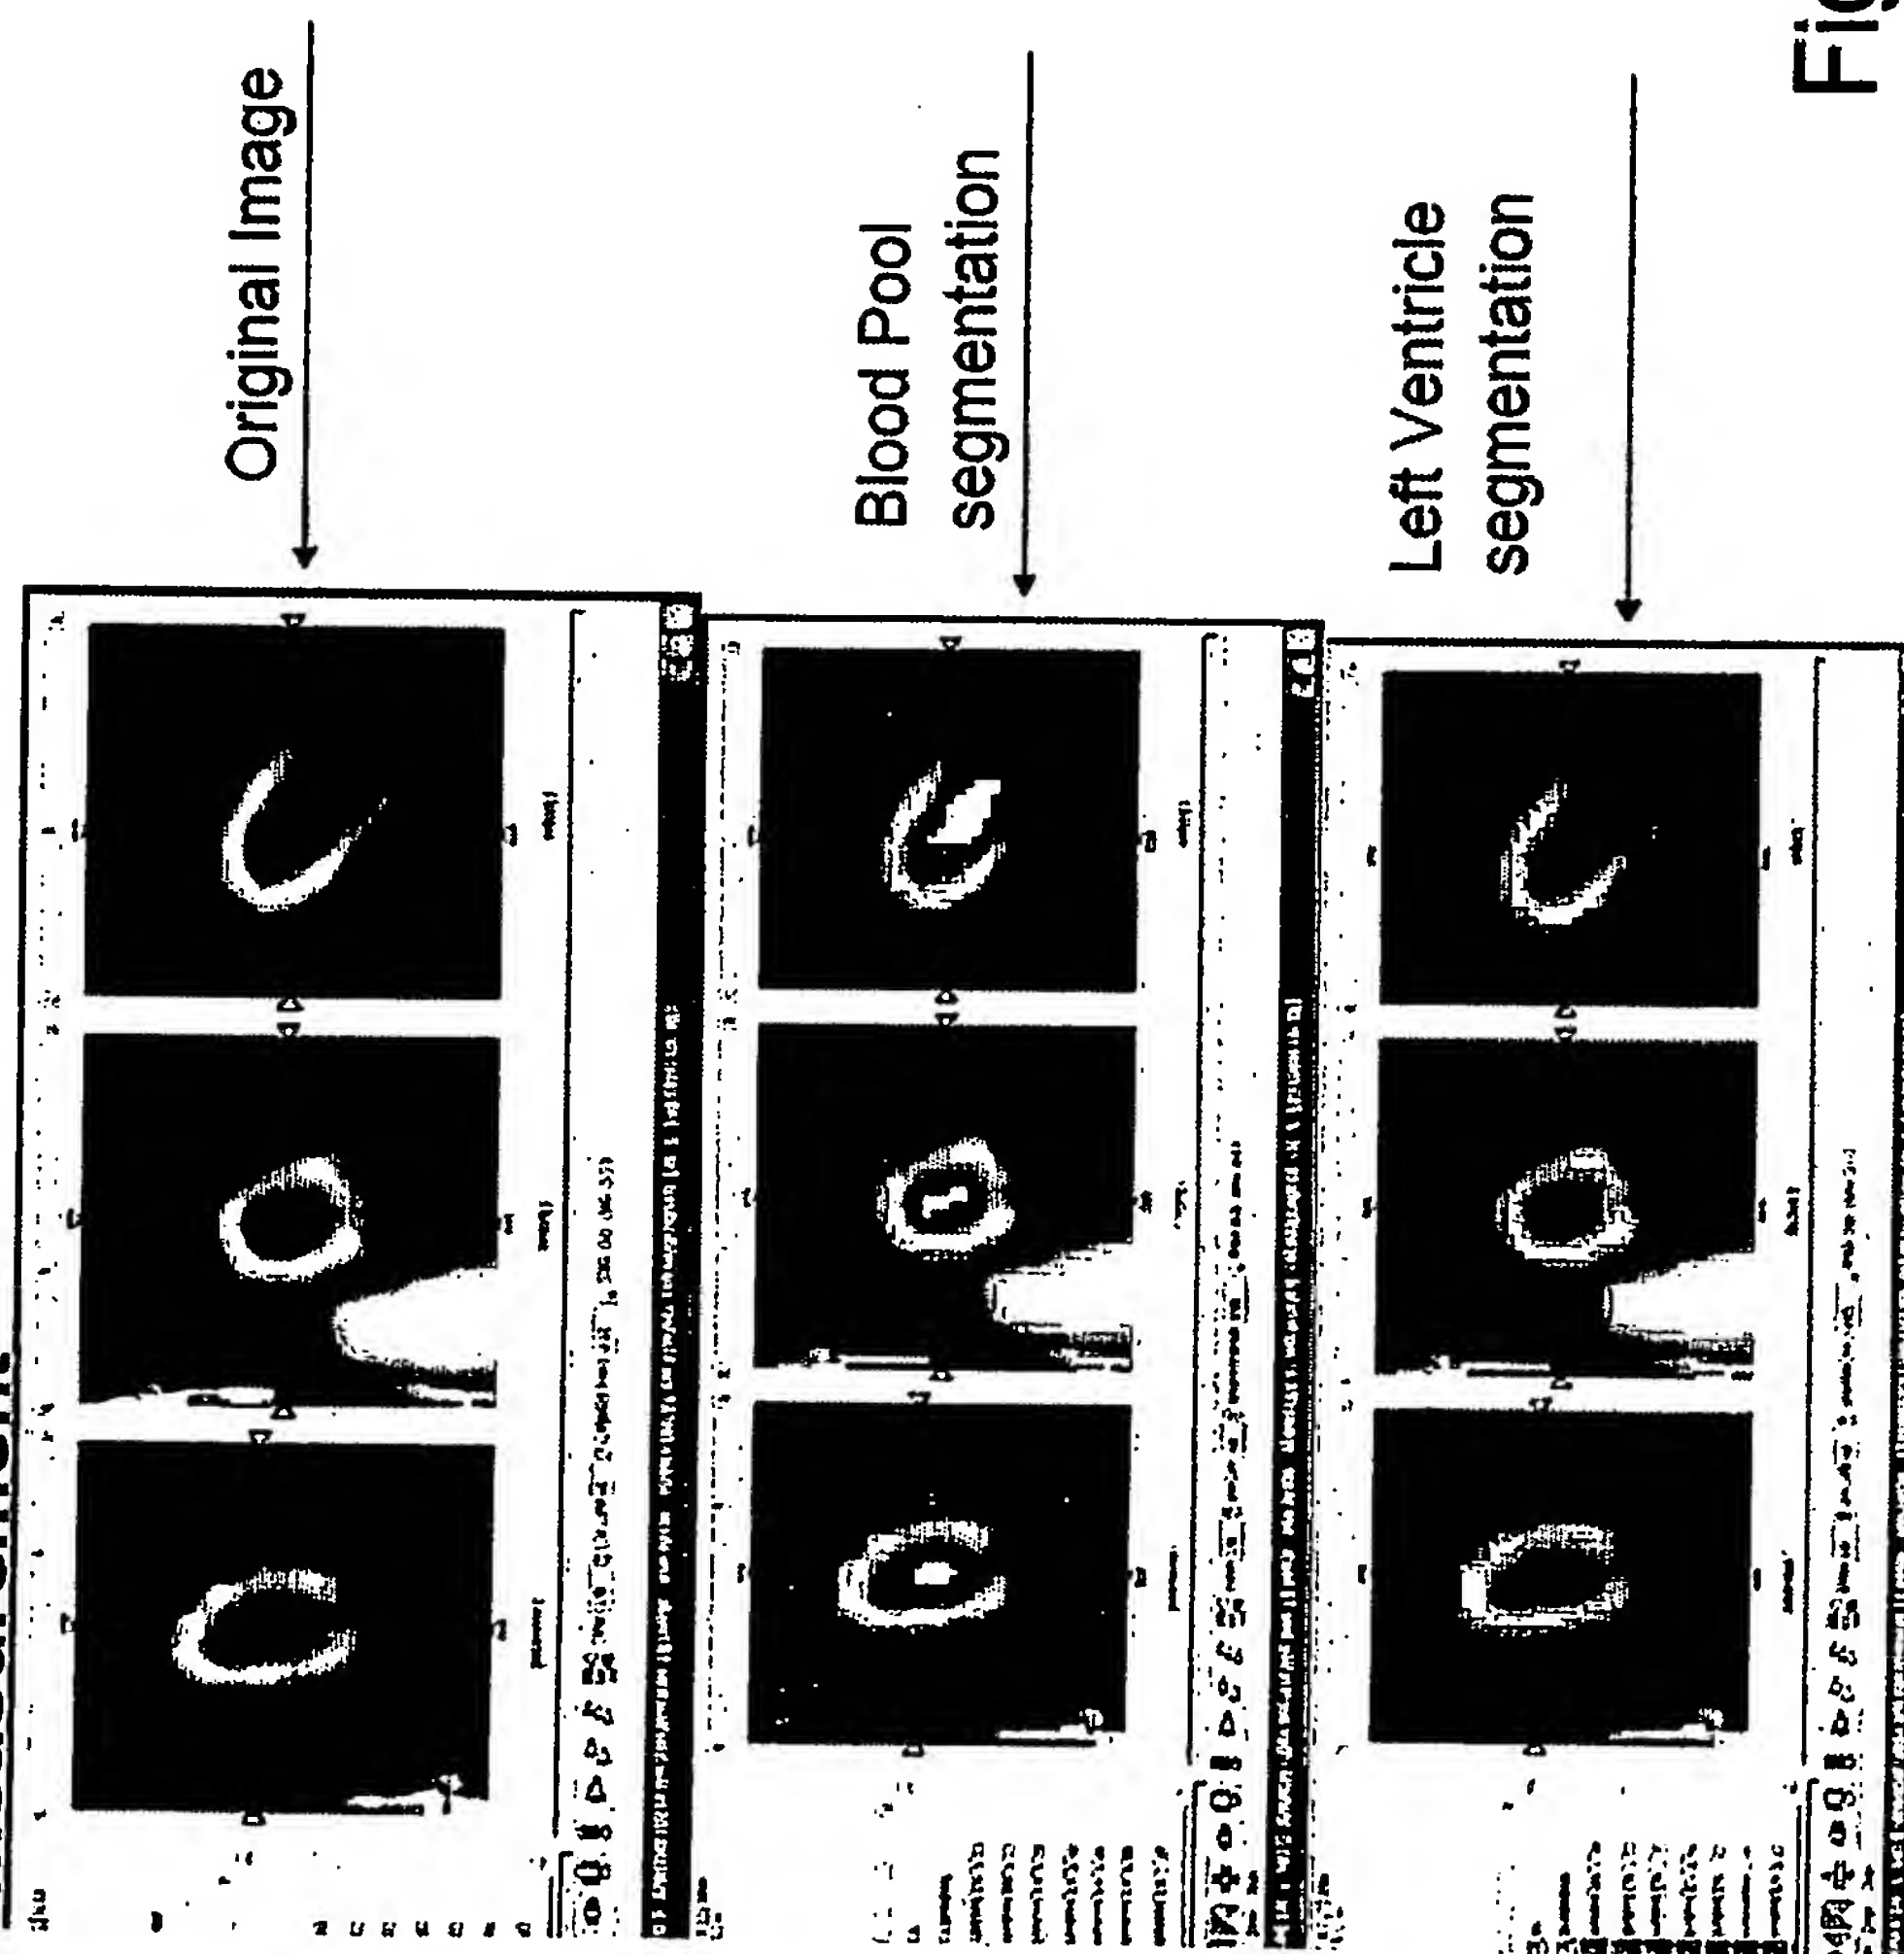


Figure 9I

Measured Kinetic curves

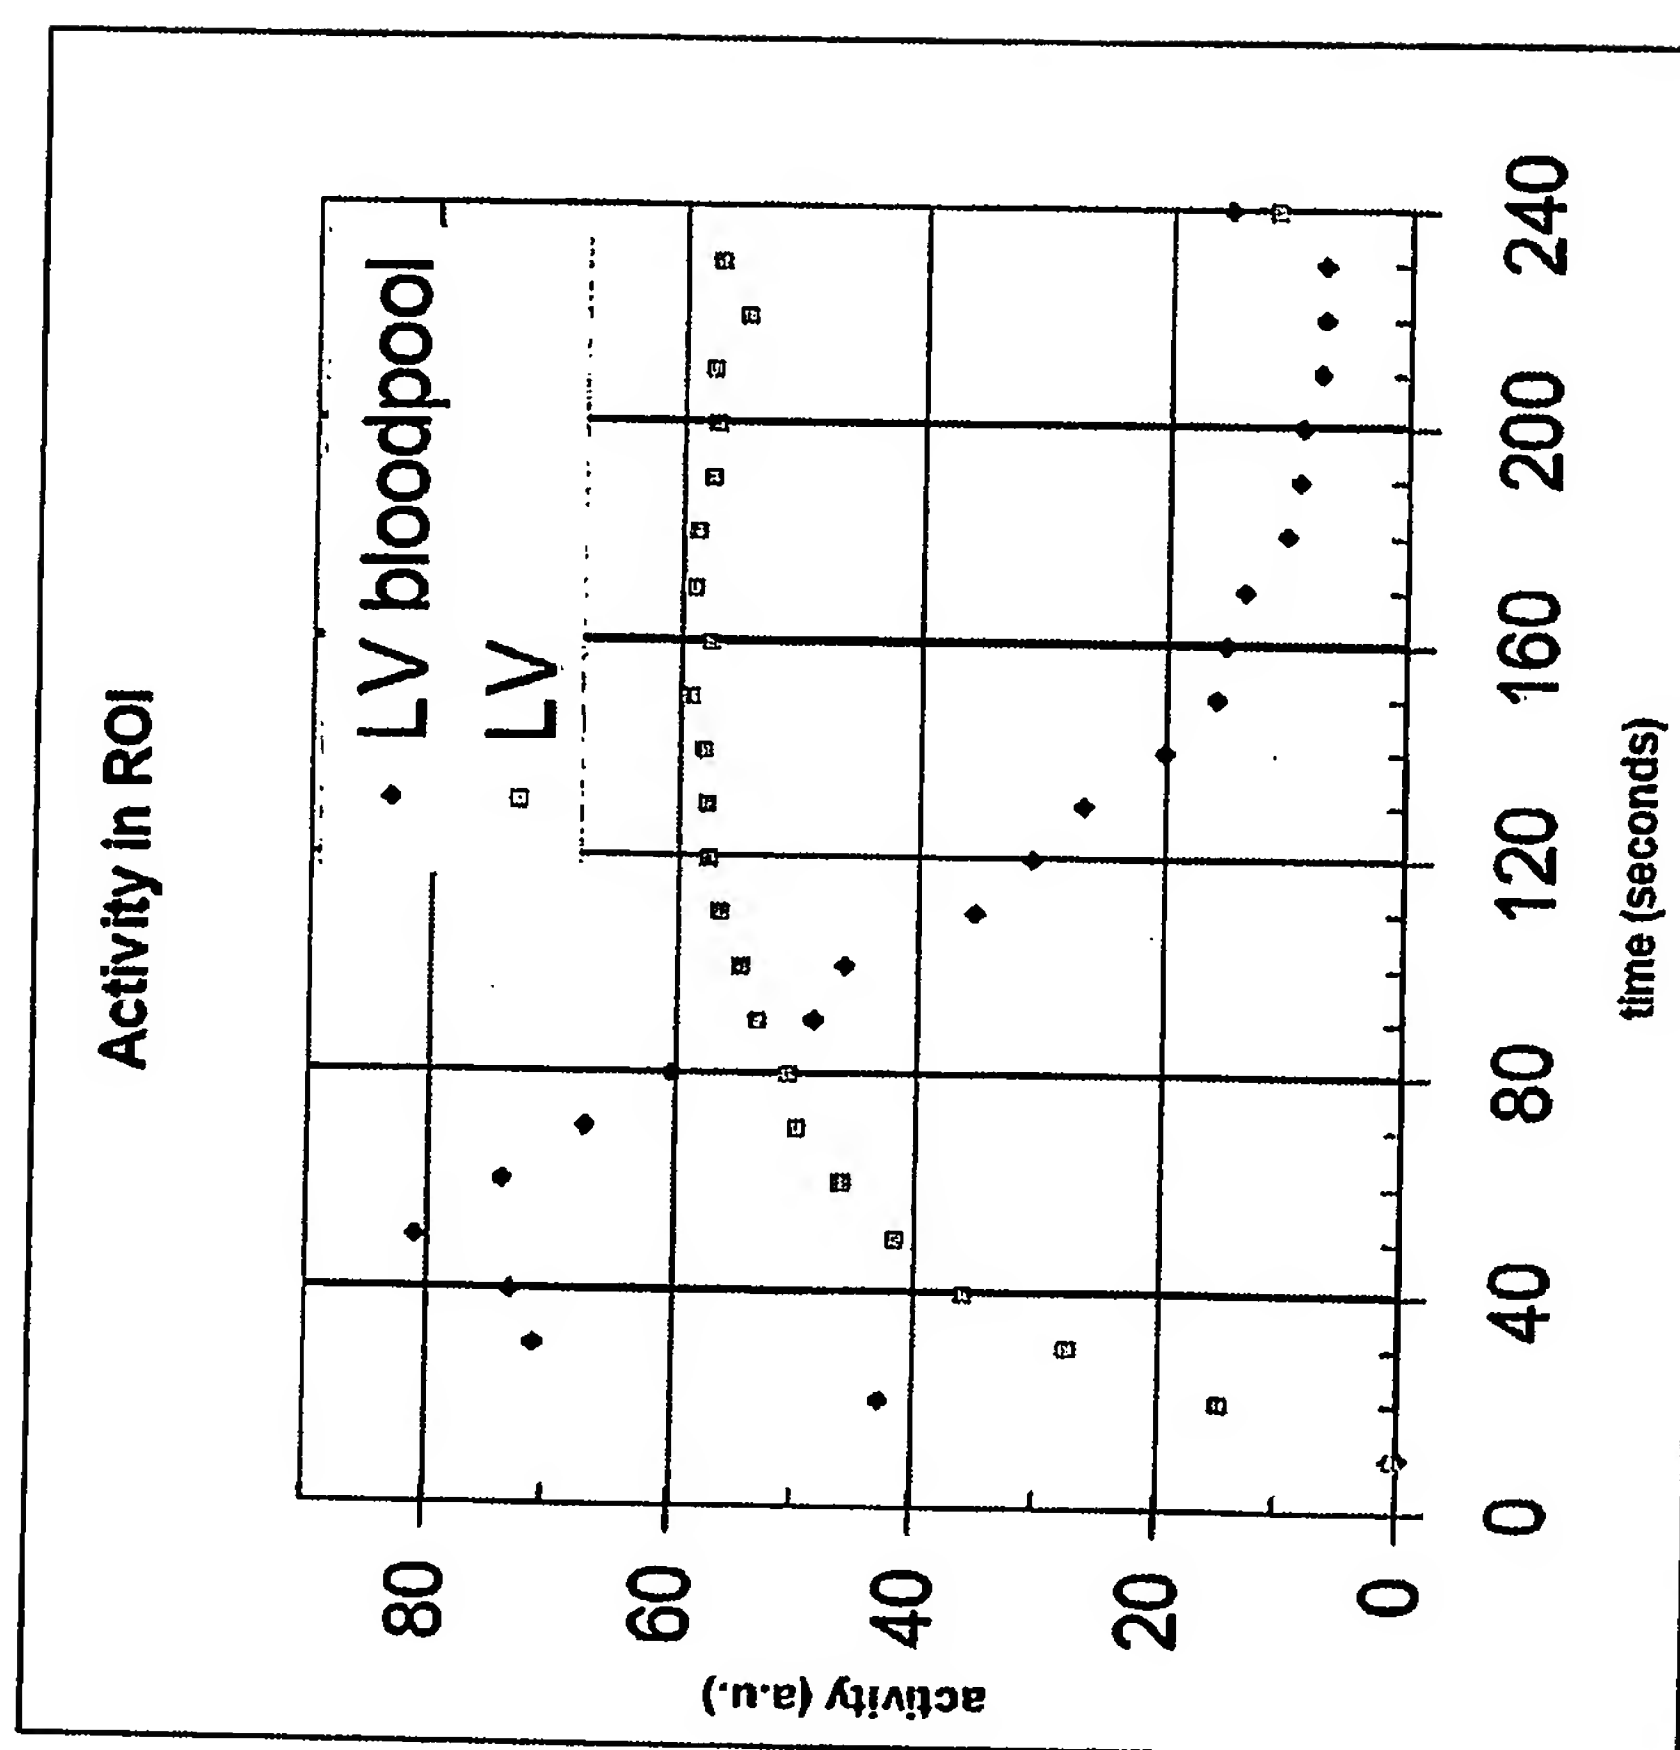


Figure 9J

Figure 10

Time (sec)	No. of events	Average rate (MHz)
0.001	56	0.056
0.002	369	
0.003	379	0.379
0.004	378	0.378
0.005	382	0.382
0.006	376	0.376
0.007	366	0.366
0.008	372	0.372
0.009	374	0.374
0.010	372	0.372
0.011	370	0.370
0.012	371	0.371
0.013	364	0.364
0.014	372	0.372
0.015	374	0.374
0.016	372	0.372
0.017	364	0.364
0.018	368	0.368
0.019	364	0.364
0.020	373	0.373
0.021	362	0.362
0.022	374	0.374
0.023	372	0.372
0.024	377	0.377
0.025	367	0.367
0.026	377	0.377
0.027	373	0.373
0.028	363	0.363
0.029	373	0.373

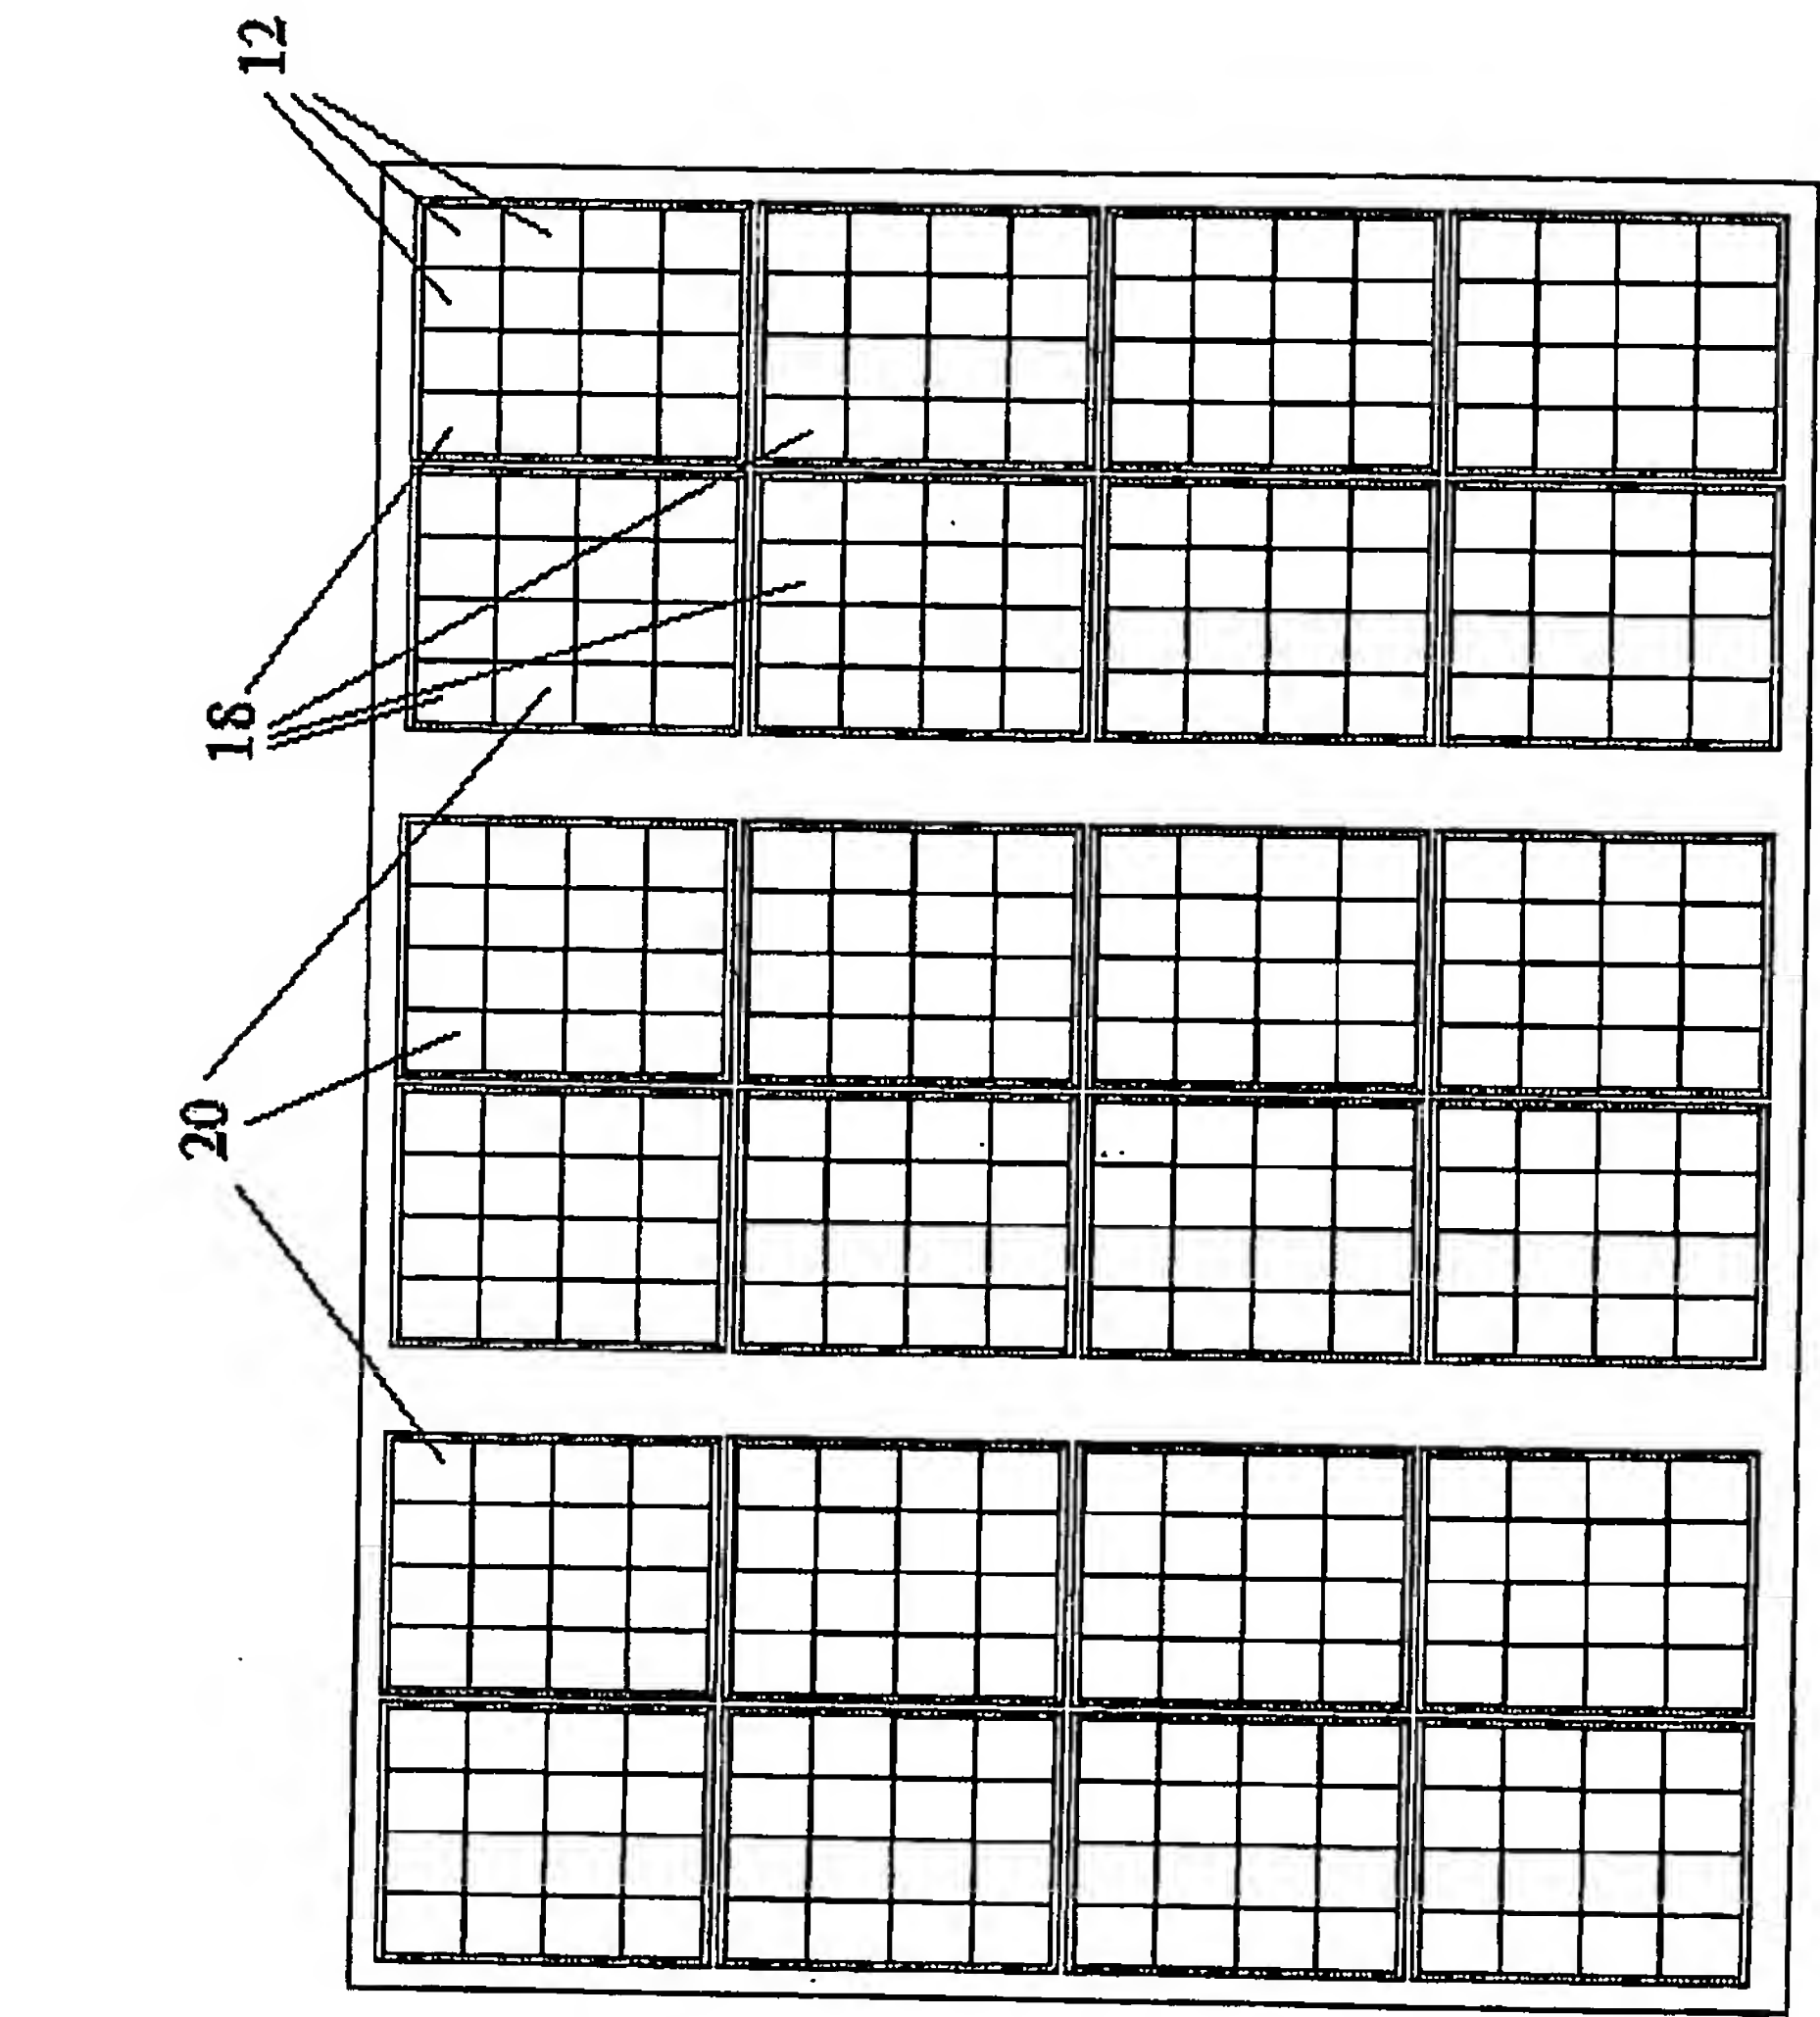


Figure 11

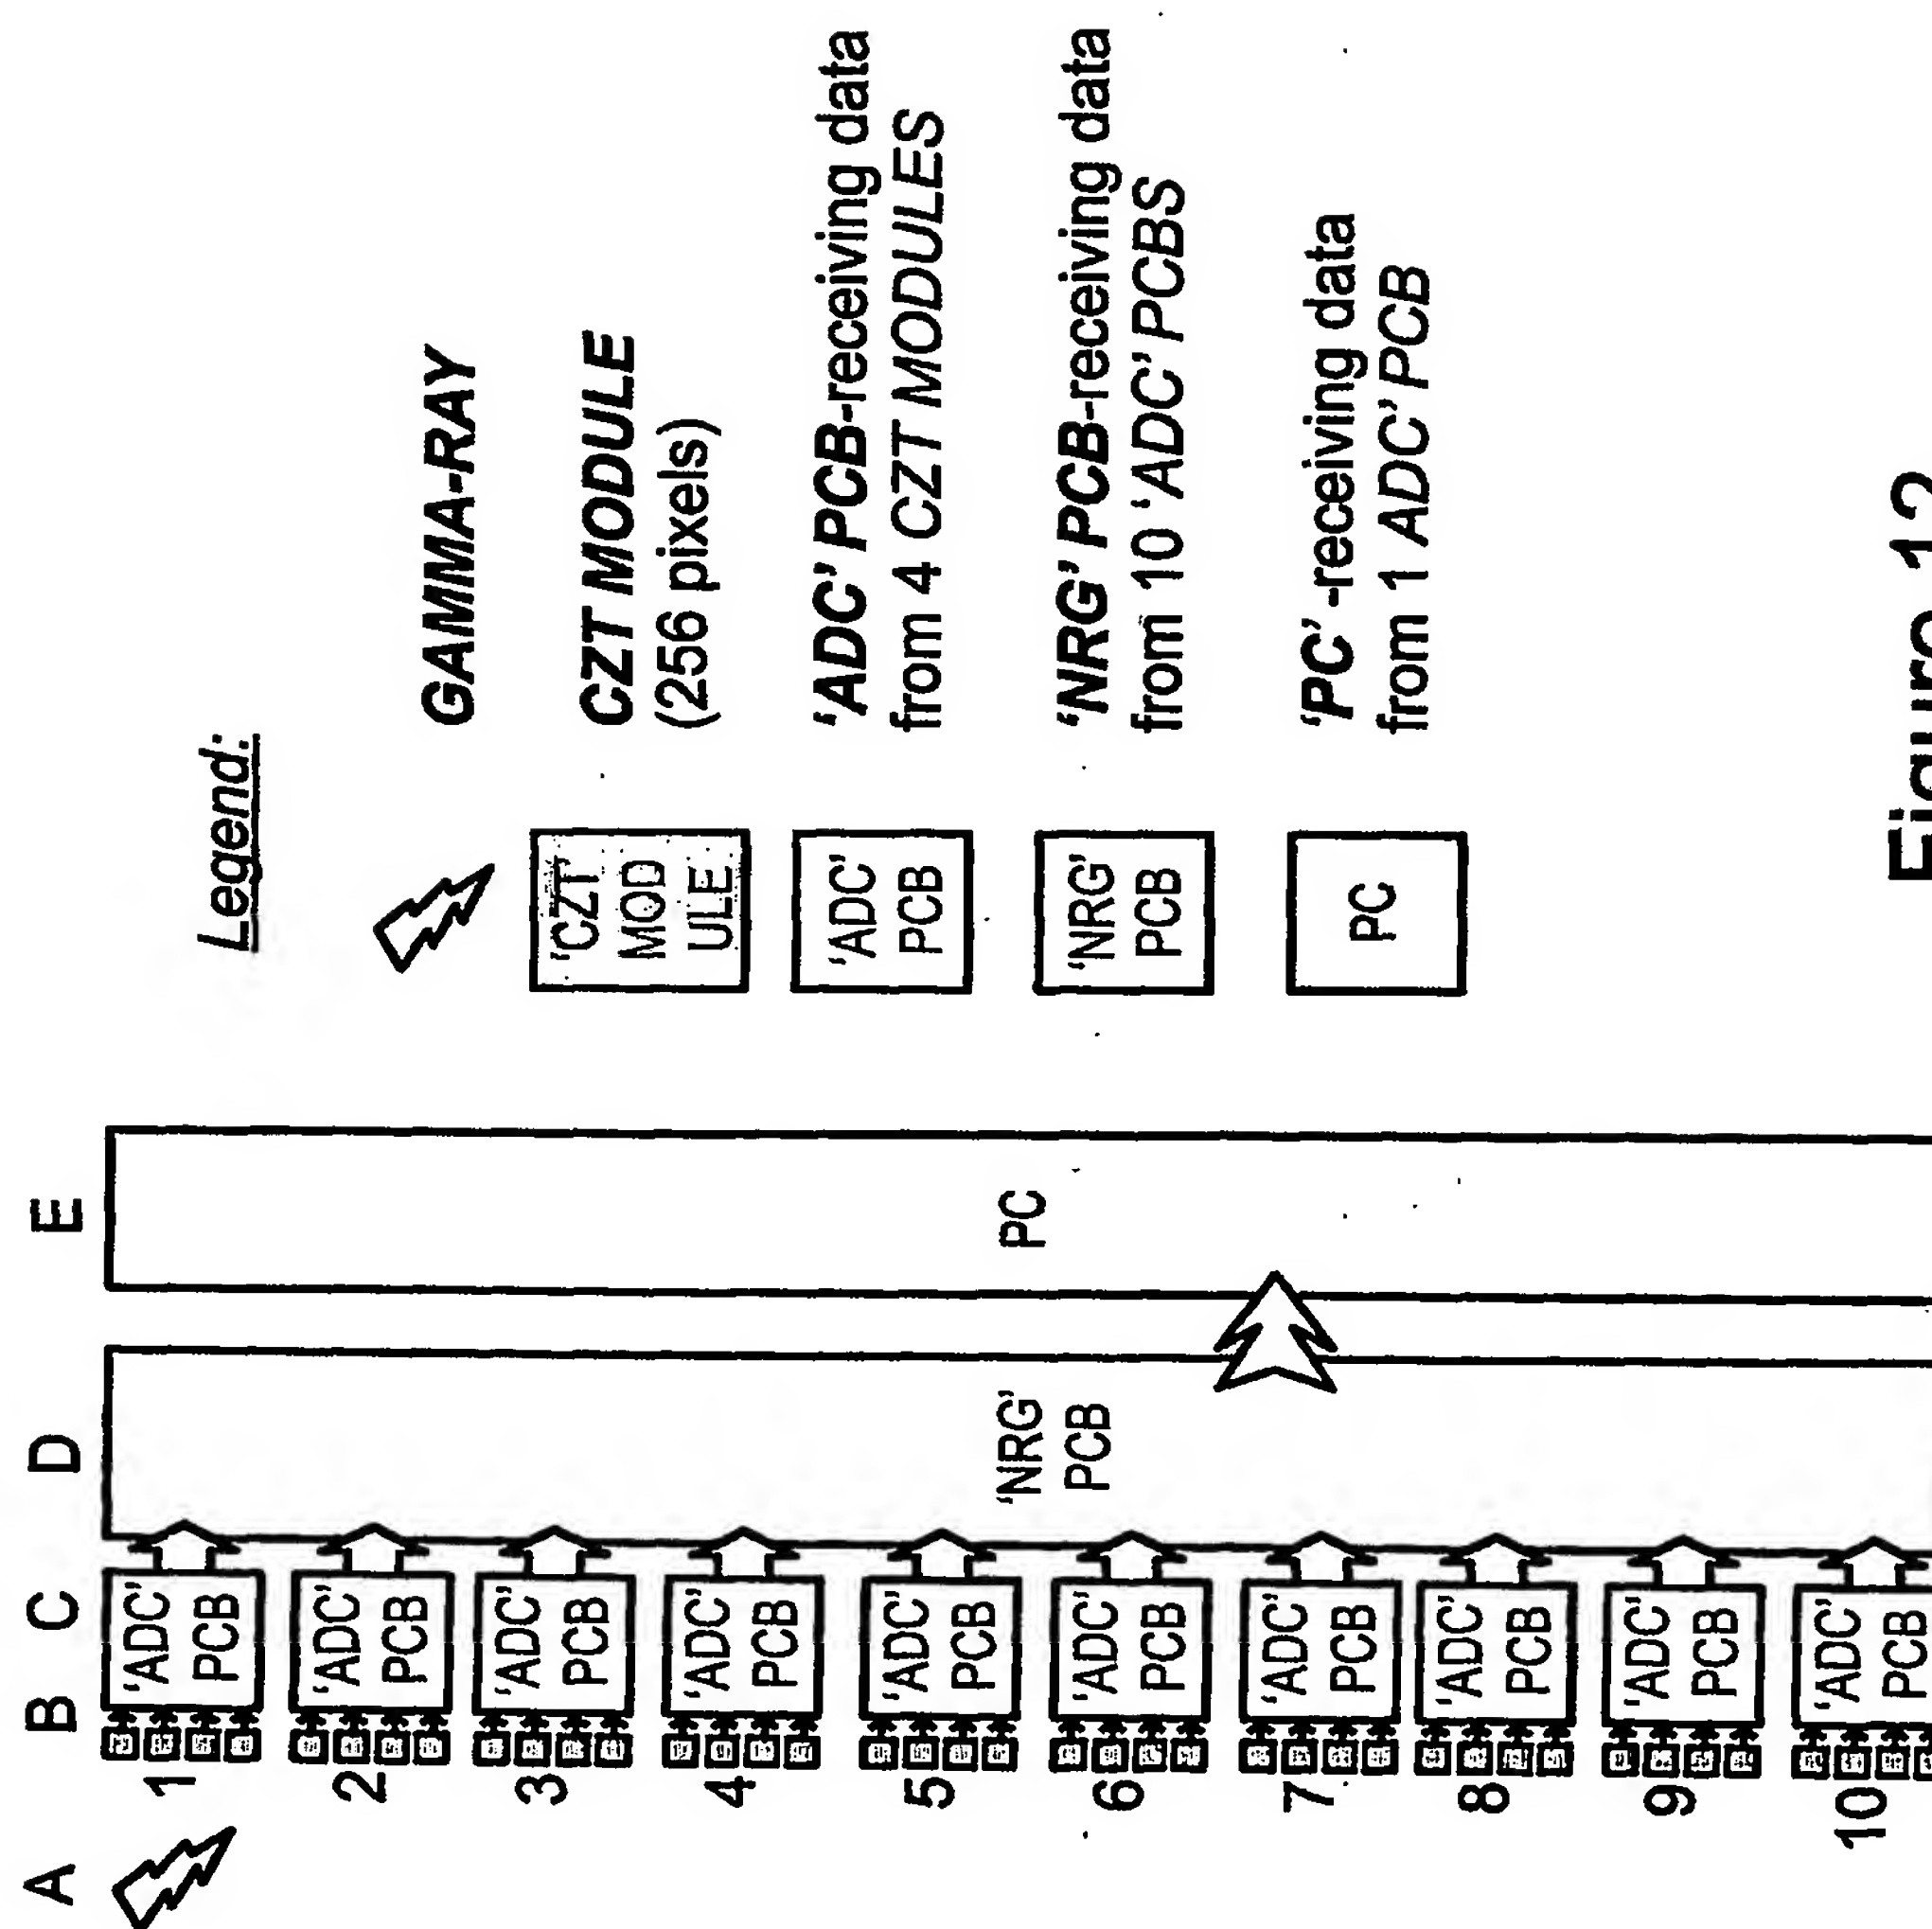


Figure 12

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



PCT



(43) International Publication Date
18 May 2007 (18.05.2007)

(10) International Publication Number
WO 2007/054935 A3

(51) International Patent Classification:
G01T 1/161 (2006.01) *G01T 1/29* (2006.01)
G01T 1/166 (2006.01)

(21) International Application Number:
PCT/IL2006/001291

(22) International Filing Date:
9 November 2006 (09.11.2006)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
PCT/IL2005/001173
9 November 2005 (09.11.2005) IL

PCT/IL2005/001215

16 November 2005 (16.11.2005) IL

172349 27 November 2005 (27.11.2005) IL

60/741,440 2 December 2005 (02.12.2005) US

60/750,287 13 December 2005 (13.12.2005) US

60/750,597 15 December 2005 (15.12.2005) US

60/750,334 15 December 2005 (15.12.2005) US

60/754,199 28 December 2005 (28.12.2005) US

PCT/IL2006/000059

15 January 2006 (15.01.2006) IL

60/763,458 31 January 2006 (31.01.2006) US

PCT/IL2006/000562 11 May 2006 (11.05.2006) IL

60/799,688 11 May 2006 (11.05.2006) US
60/800,845 17 May 2006 (17.05.2006) US
60/800,846 17 May 2006 (17.05.2006) US
60/816,970 28 June 2006 (28.06.2006) US
PCT/IL2006/000834 19 July 2006 (19.07.2006) IL
PCT/IL2006/000840 19 July 2006 (19.07.2006) IL

(71) Applicant (*for all designated States except US*): **SPECTRUM DYNAMICS LLC** [US/US]; 30 Ramland Road South, Orangeburg, New York 10962 (US).

(72) Inventors; and


(75) Inventors/Applicants (*for US only*): **ROUSSO, Benny** [IL/IL]; 12 Henri Bergson Street, 75801 Rishon-lezion (IL). **ZIV, Omer** [IL/IL]; 3 Einstein Street, 76470 Rechovot (IL). **NAGLER, Michael** [IL/IL]; 4 Avshalom Haviv Street, 69495 Tel-aviv (IL). **BEN-HAIM, Shlomo** [IL/IL]; 8 Efroni Street, 38900 Caesarea (IL).

(74) Agents: **G. E. EHRlich (1995) LTD.** et al.; 11 Menachem Begin Street, 52 521 Ramat Gan (IL).

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS,

[Continued on next page]

(54) Title: DYNAMIC SPECT CAMERA

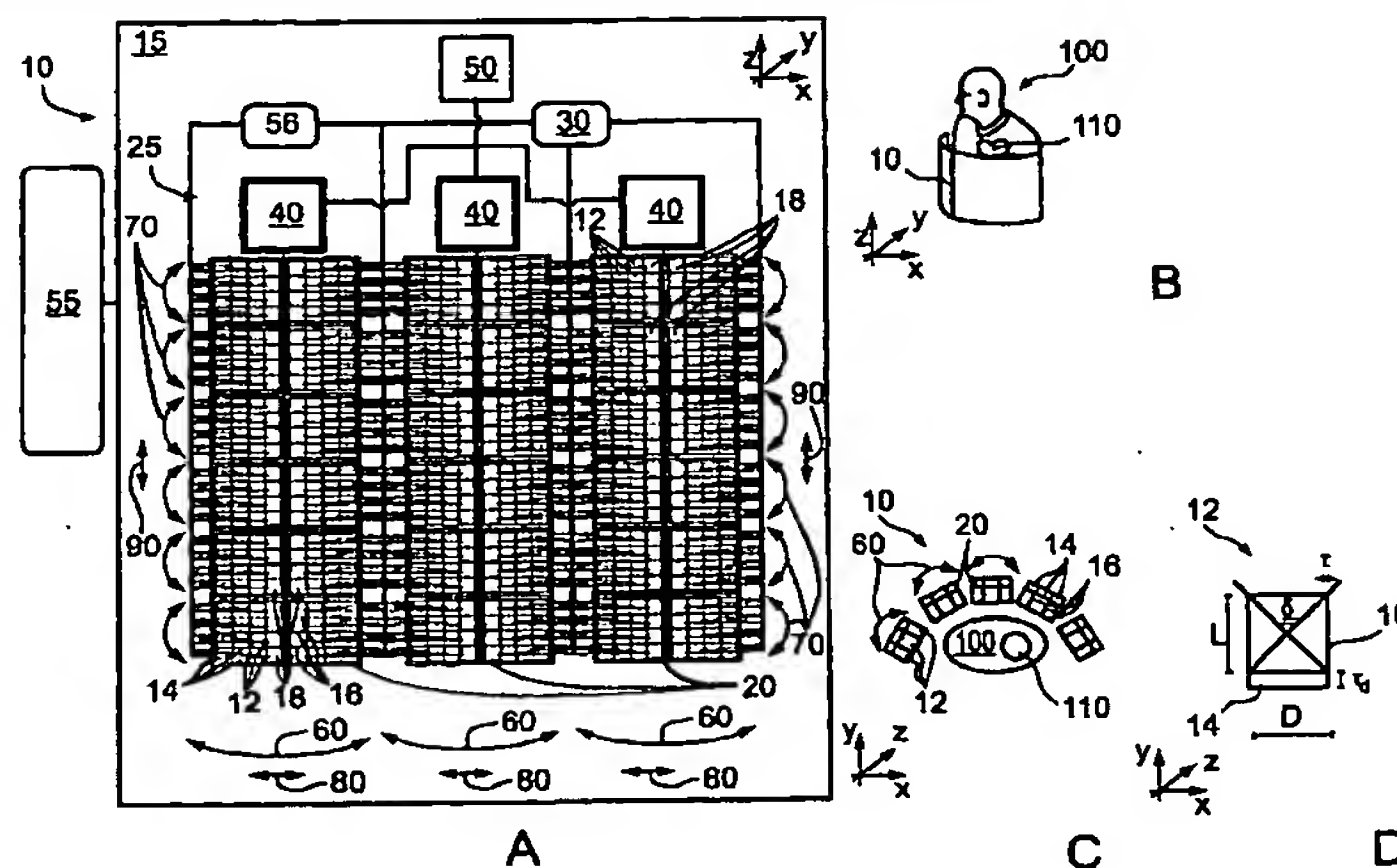

(57) Abstract: A dynamic SPECT camera is provided, comprising, a plurality of single-pixel detectors, a timing mechanism, in communication with each single-pixel detector, configured for enabling time-binning of the radioactive emissions impinging upon each single-pixel detector to time periods not greater than substantially 30 seconds, and a position-tracker, configured for providing information on the position and orientation of each detecting unit, with respect to the overall structure, substantially at all times, during the individual motion, the dynamic SPECT camera being configured for acquiring a tomographic reconstruction image of a region of interest of about 15 X 15 X 15 cubic centimeters, during an acquisition time of 30 seconds, at a spatial resolution of at least 10 X 10 X 10 cubic millimeter. The dynamic camera is configured for very short damping time, and may further acquire images in a stationary mode, with no motion. It is further configured for time binning at dynamically varying time-bin lengths, dynamically determining a spectral energy bin for each detecting unit, and employing an anatomic construction of voxels in the imaging and reconstruction.

WO 2007/054935 A3



LT, LU, LV, LY, MA, MD, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT,

(88) Date of publication of the international search report:
22 November 2007

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

INTERNATIONAL SEARCH REPORT

International application No
PCT/IL2006/001291

A. CLASSIFICATION OF SUBJECT MATTER

INV. G01T1/161 G01T1/166 G01T1/29

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

G01T

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, INSPEC, COMPENDEX

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 6 242 743 B1 (DEVITO RAYMOND P [US] ET AL) 5 June 2001 (2001-06-05) cited in the application figures column 15, line 33 - line 38 column 15, line 47 - line 55 column 17, line 56 - line 60 column 18, line 45 - line 59 column 19, line 5 - line 17 column 19, line 18 - line 38 column 24, line 9 - line 50 column 25, line 14 - line 39 claims 1,5,6,67	1,73,131
A	GB 2 031 142 A (SHAW R) 16 April 1980 (1980-04-16) page 4, line 48 - line 57; figures ----- -/--	1,73,131

☒ Further documents are listed in the continuation of Box C.☒ See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

16 March 2007

Date of mailing of the international search report

02.07.07

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Eberle, Katja

INTERNATIONAL SEARCH REPORT

International application No

PCT/IL2006/001291

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	<p>A01 T ET AL: "Absolute quantitation of regional myocardial blood flow of rats using dynamic pinhole SPECT"</p> <p>2002 IEEE NUCLEAR SCIENCE SYMPOSIUM CONFERENCE RECORD. / 2002 IEEE NUCLEAR SCIENCE SYMPOSIUM AND MEDICAL IMAGING CONFERENCE. NORFOLK, VA, NOV. 10 - 16, 2002, IEEE NUCLEAR SCIENCE SYMPOSIUM CONFERENCE RECORD, NEW YORK, NY : IEEE, US, vol. VOL. 3 OF 3, 10 November 2002 (2002-11-10), pages 1780-1783, XP010663867</p> <p>ISBN: 0-7803-7636-6</p> <p>abstract; figures</p>	1,73,131
A	<p>US 2004/204646 A1 (NAGLER MICHAEL [IL] ET AL) 14 October 2004 (2004-10-14)</p> <p>figures</p> <p>page 5, paragraph 96</p> <p>page 6, paragraph 101 - page 7, paragraph 110</p> <p>page 7, paragraph 121 - paragraph 123</p> <p>page 8, paragraph 137</p>	73
A	<p>US 5 846 513 A1 (CARROLL ROBERT G [US] ET AL CARROLL ROBERT G [US] ET AL) 8 December 1998 (1998-12-08)</p> <p>column 4, line 61 - column 6, line 60; figures</p>	73

INTERNATIONAL SEARCH REPORT

International application No.
PCT/IL2006/001291

Box II Observations where certain claims were found unsearchable (Continuation of Item 2 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box III Observations where unity of invention is lacking (Continuation of Item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-93, 131

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1-93, 131

A method of dynamic SPECT data acquisition and a dynamic SPECT camera characterised by the timing mechanism enabling time-binning of radioactive emissions to time periods not greater than 30 seconds and an acquisition time for a tomographic reconstruction image of 300 seconds and an intracorporeal dynamic SPECT camera.

2. claim: 94

A dynamic SPECT camera of short damping time.

3. claims: 95-103

A stationary SPECT camera.

4. claims: 104, 105, 132

A dynamic SPECT camera for time binning at dynamically varying time-bin lengths.

5. claims: 106-116, 133

A method and a dynamic SPECT camera for dynamically determining a spectral energy bin for each detecting unit.

6. claims: 117-130

A method for anatomic construction of voxels.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/IL2006/001291

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 6242743	B1	05-06-2001	NONE
GB 2031142	A	16-04-1980	NONE
US 2004204646	A1	14-10-2004	NONE
US 5846513	A1		NONE